

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111822\
 Data File : VW029121.D
 Acq On : 18 Nov 2022 16:24
 Operator : SY/MD
 Sample : N5687-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCE3

Quant Time: Nov 18 23:34:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	271375	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	251751	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	109194	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	73558	4.446	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.000%	
7) Chloroethane-d5	1.568	69	67324	4.629	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.600%	
11) 1,1-Dichloroethene-d2	2.108	63	105300	3.493	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.800%	
20) 2-Butanone-d5	3.902	46	116570	42.091	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.180%	
24) Chloroform-d	4.342	84	171936	5.062	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.030	65	80117	5.242	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.800%	
32) Benzene-d6	5.047	84	350301	4.662	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.200%	
36) 1,2-Dichloropropane-d6	6.066	67	109191	5.204	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.000%	
41) Toluene-d8	7.313	98	316486	4.679	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.600%	
43) trans-1,3-Dichloroprop...	7.622	79	32351	4.727	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.091	63	148970	50.996	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	102.000%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	81802	5.623	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	112.400%	
66) 1,2-Dichlorobenzene-d4	11.615	152	110527	5.658	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.200%	
Target Compounds						Qvalue
3) Chloromethane	1.240	50	4668	0.249	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029121.D
Acq On : 18 Nov 2022 16:24
Operator : SY/MD
Sample : N5687-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE3

Quant Time: Nov 18 23:34:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 04:35:43 2022
Response via : Initial Calibration

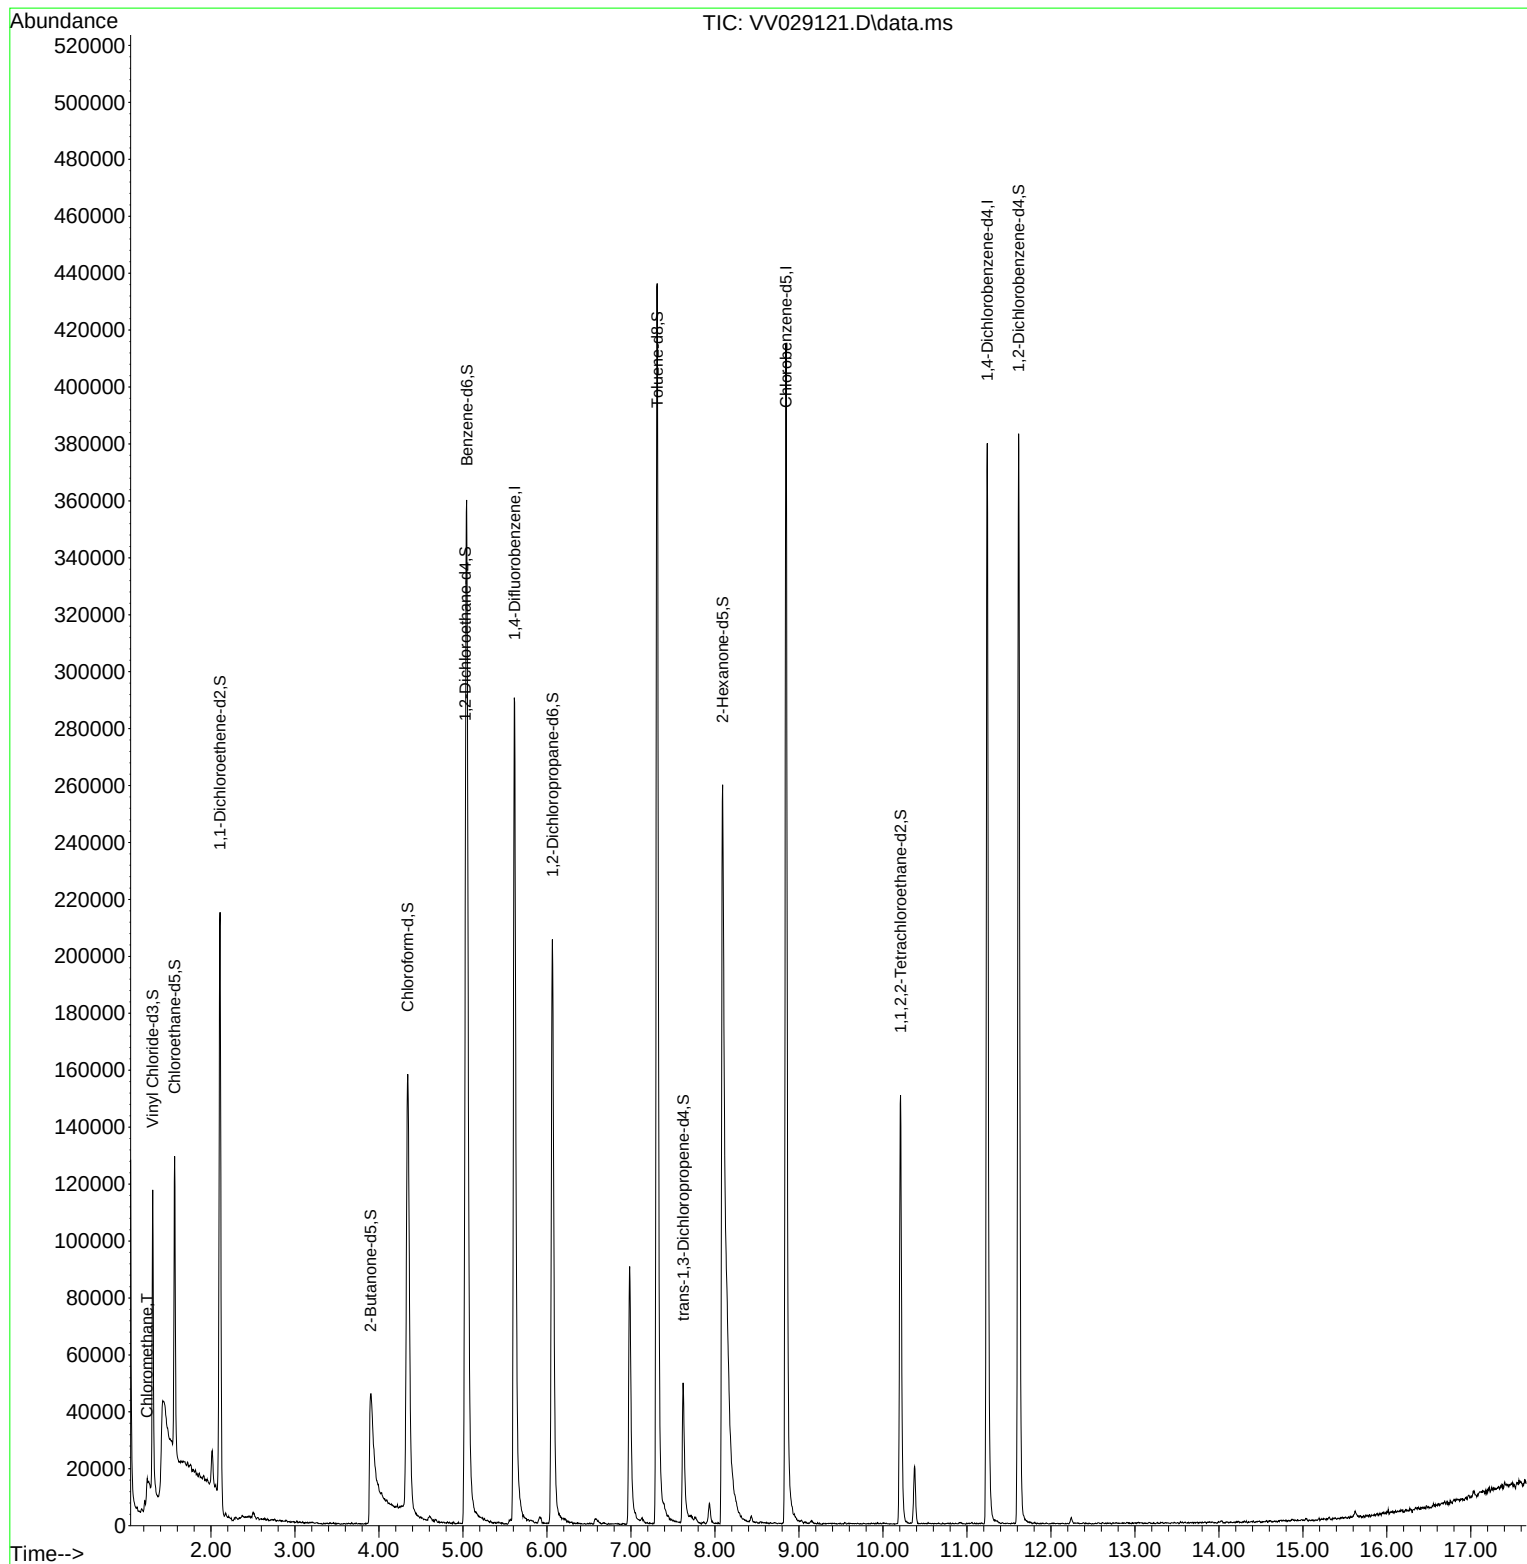

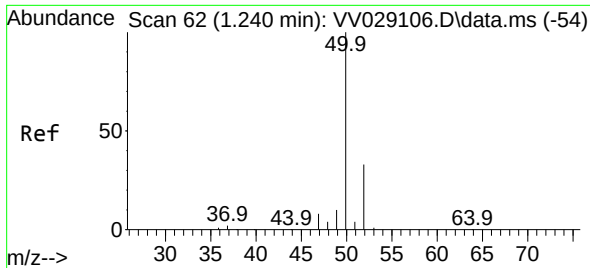

#3
 Chloromethane
 Concen: 0.249 ug/L
 RT: 1.240 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: VV029121.D
 Acq: 18 Nov 2022 16:24

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCE3

Tgt Ion: 50 Resp: 4668
 Ion Ratio Lower Upper
 50 100
 52 28.5 23.7 43.9

