

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111822\
 Data File : VW029152.D
 Acq On : 19 Nov 2022 05:42
 Operator : SY/MD
 Sample : N5666-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB28

Quant Time: Nov 19 06:06:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	290050	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	265912	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	120812	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67718	3.830	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	76.600%	
7) Chloroethane-d5	1.568	69	64707	4.163	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.200%	
11) 1,1-Dichloroethene-d2	2.108	63	93692	2.907	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.200%#	
20) 2-Butanone-d5	3.892	46	215203	72.703	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	145.400%#	
24) Chloroform-d	4.342	84	167152	4.604	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
26) 1,2-Dichloroethane-d4	5.030	65	82113	5.027	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.600%	
32) Benzene-d6	5.047	84	333464	4.201	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.000%	
36) 1,2-Dichloropropane-d6	6.066	67	108768	4.908	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.310	98	287887	4.029	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.600%	
43) trans-1,3-Dichloroprop...	7.622	79	31824	4.402	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.000%	
46) 2-Hexanone-d5	8.085	63	159891	51.820	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.640%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	81927	5.332	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.600%	
66) 1,2-Dichlorobenzene-d4	11.615	152	109778	5.079	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.600%	
Target Compounds						
13) Acetone	2.188	43	9327	4.898	ug/L	94
15) Methyl Acetate	2.439	43	2934	0.635	ug/L #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029152.D
Acq On : 19 Nov 2022 05:42
Operator : SY/MD
Sample : N5666-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB28

Quant Time: Nov 19 06:06:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 04:35:43 2022
Response via : Initial Calibration

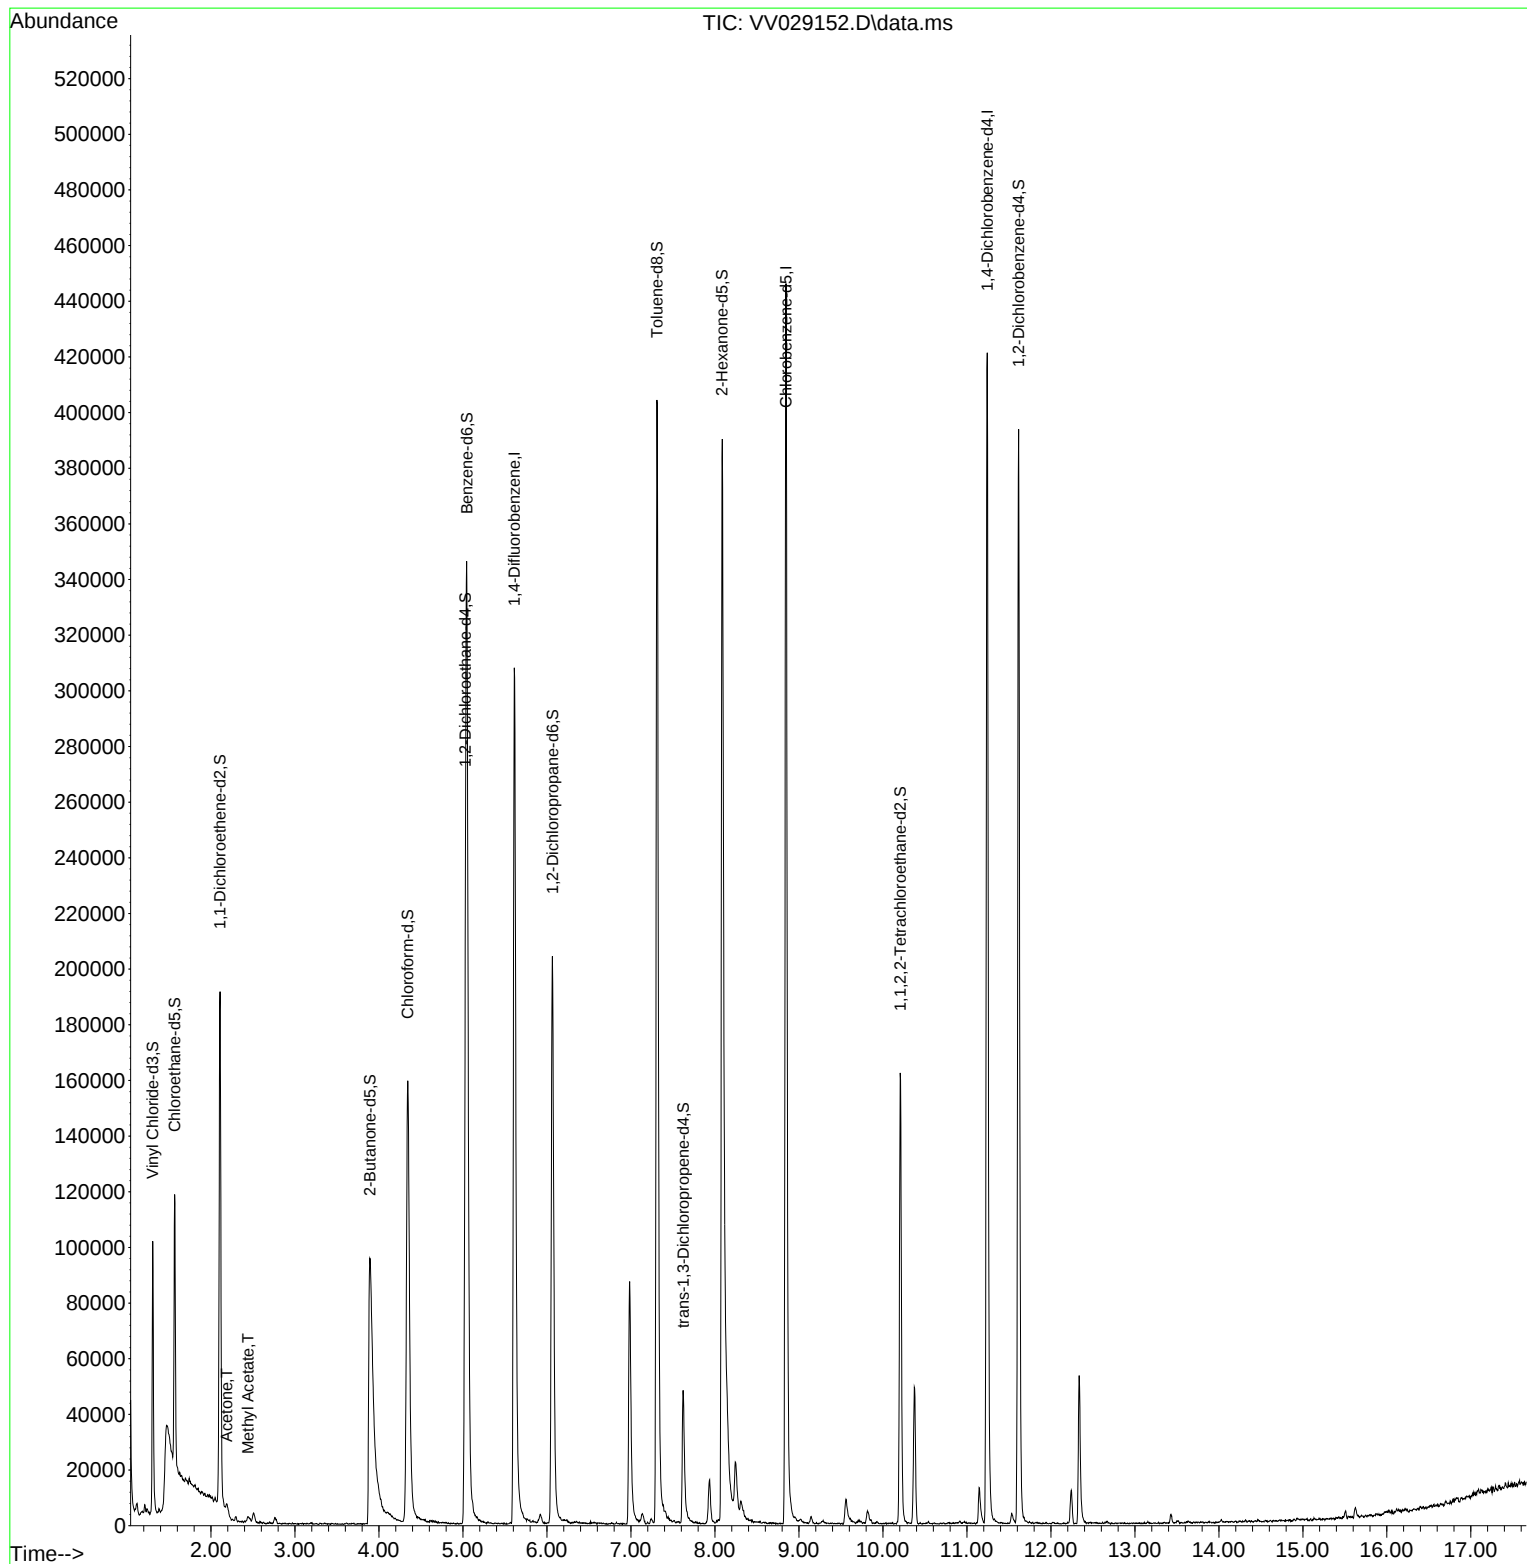

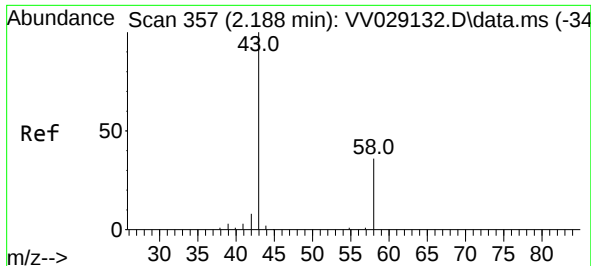

#13

Acetone

Concen: 4.898 ug/L

RT: 2.188 min Scan# 357

Delta R.T. -0.000 min

Lab File: VV029152.D

Acq: 19 Nov 2022 05:42

Instrument :

MSVOA_V

ClientSampleId :





BHB28

Tgt Ion: 43 Resp: 9327

Ion Ratio Lower Upper

43 100

58 25.2 0.0 56.6

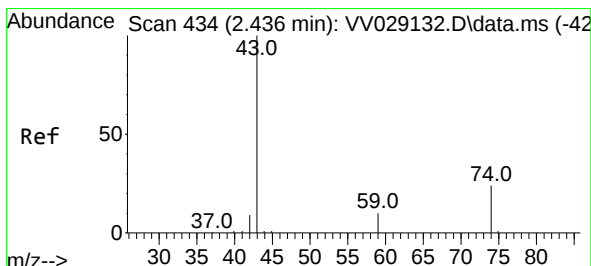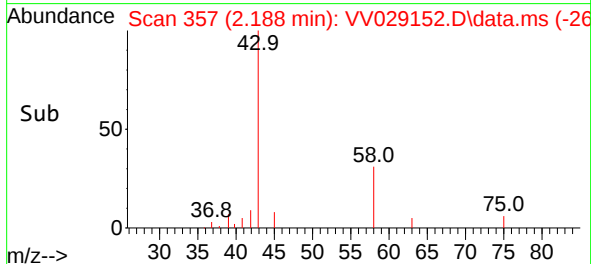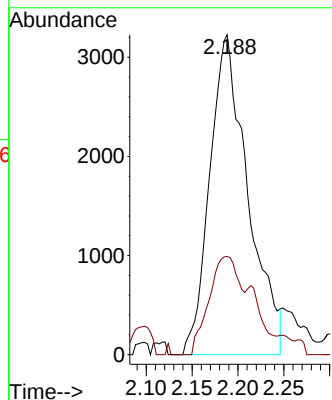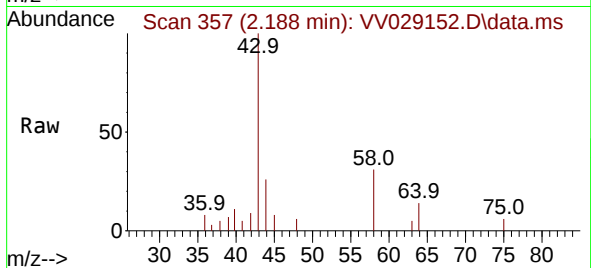

#15

Methyl Acetate

Concen: 0.635 ug/L

RT: 2.439 min Scan# 435

Delta R.T. -0.000 min

Lab File: VV029152.D

Acq: 19 Nov 2022 05:42

Tgt Ion: 43 Resp: 2934

Ion Ratio Lower Upper

43 100

74 15.7 24.6 37.0#

