

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029153.D
 Acq On : 19 Nov 2022 06:06
 Operator : SY/MD
 Sample : N5666-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB29

Quant Time: Nov 20 00:49:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Nov 20 00:44:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	296258	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	270519	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	126677	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	66149	3.662	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.568	69	62221	3.919	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.400%
11) 1,1-Dichloroethene-d2	2.105	63	93056	2.827	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.600%#
20) 2-Butanone-d5	3.896	46	209321	69.234	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	138.460%#
24) Chloroform-d	4.343	84	162743	4.389	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.031	65	80219	4.808	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	5.047	84	331223	4.102	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	6.066	67	104443	4.632	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.600%
41) Toluene-d8	7.310	98	281294	3.870	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.400%
43) trans-1,3-Dichloroprop...	7.622	79	31023	4.219	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.400%
46) 2-Hexanone-d5	8.088	63	157019	50.023	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.040%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	82643	5.287	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.800%
66) 1,2-Dichlorobenzene-d4	11.616	152	109232	4.820	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						Qvalue
15) Methyl Acetate	2.449	43	3582	0.759	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029153.D
Acq On : 19 Nov 2022 06:06
Operator : SY/MD
Sample : N5666-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB29

Quant Time: Nov 20 00:49:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Nov 20 00:44:38 2022
Response via : Initial Calibration

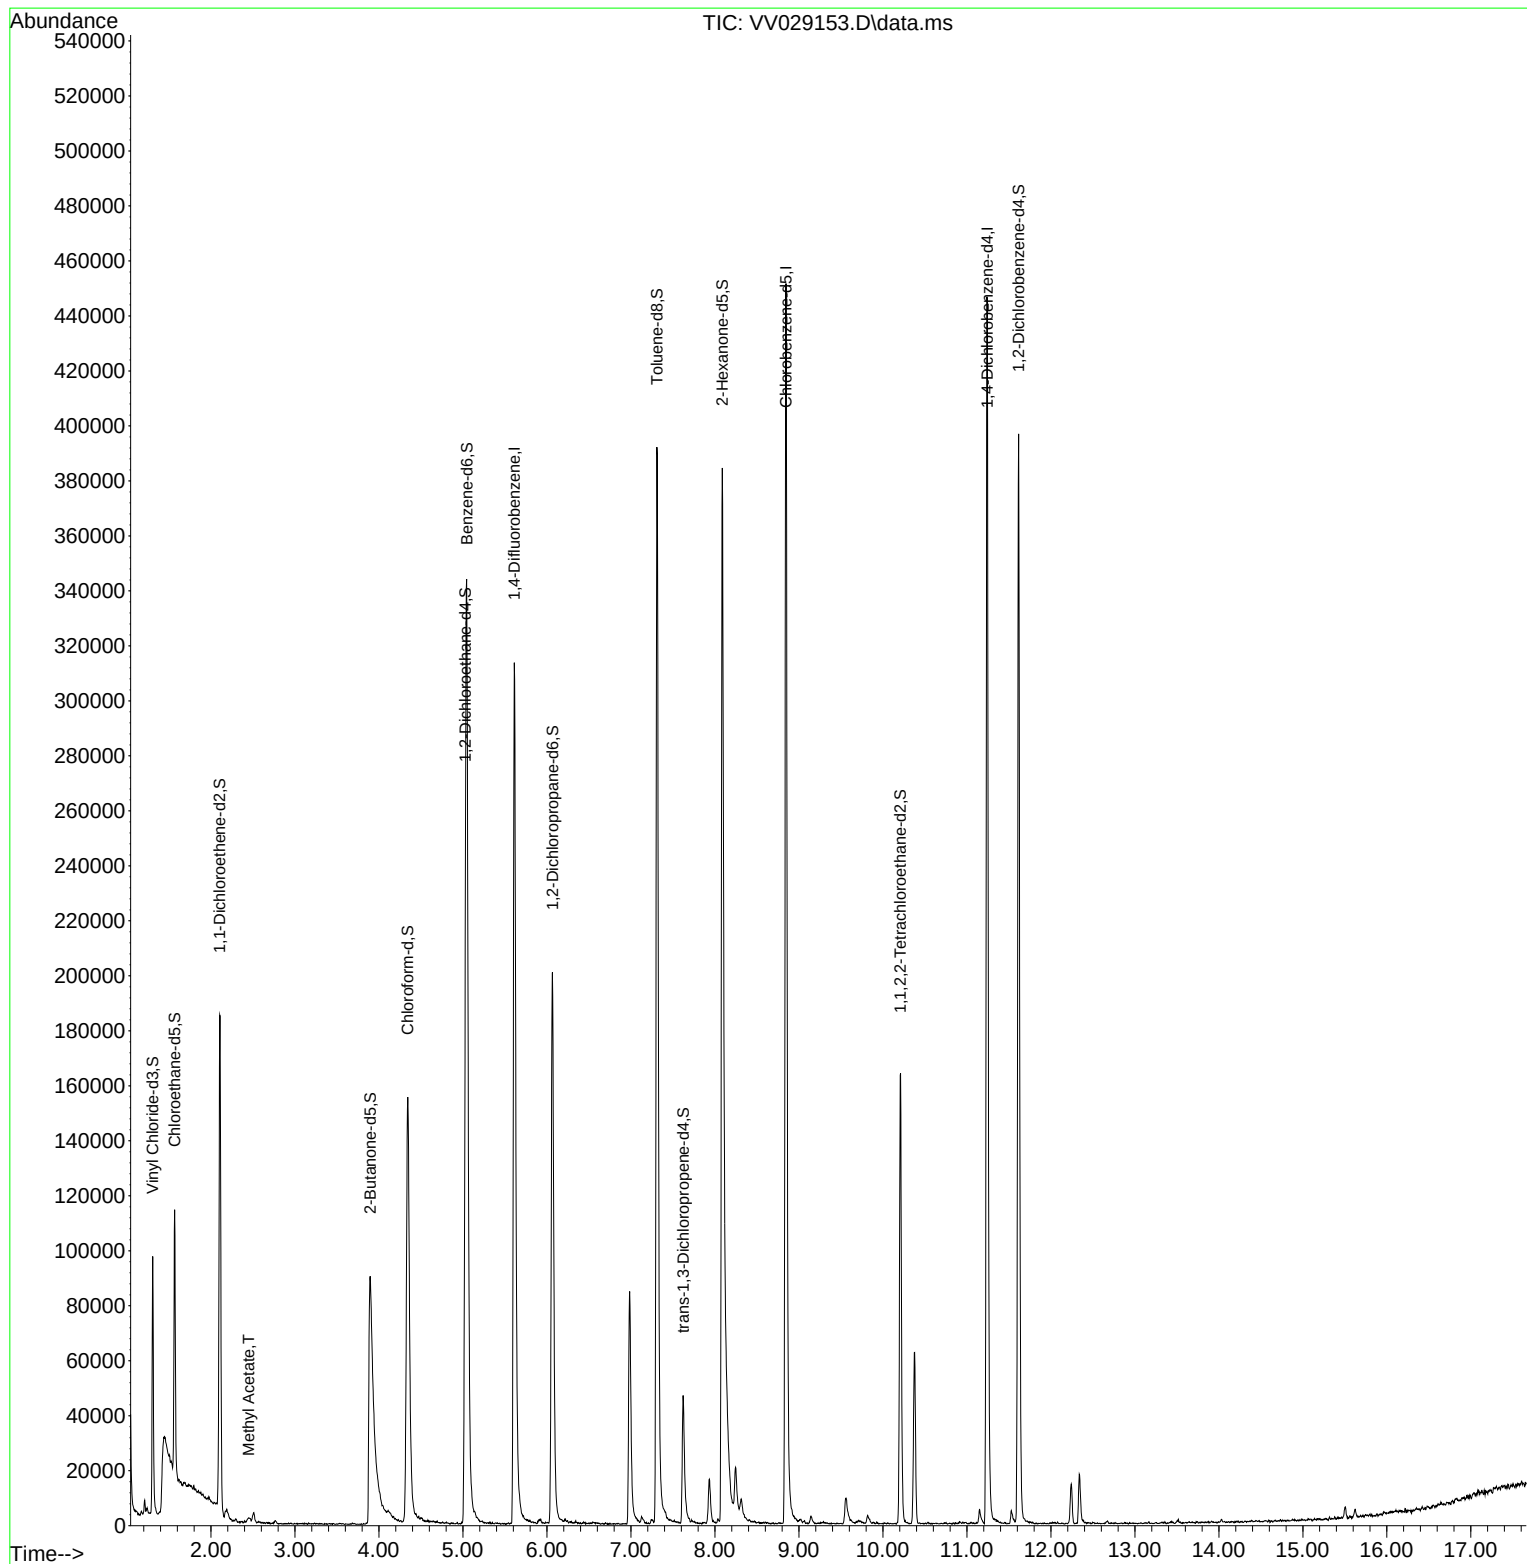

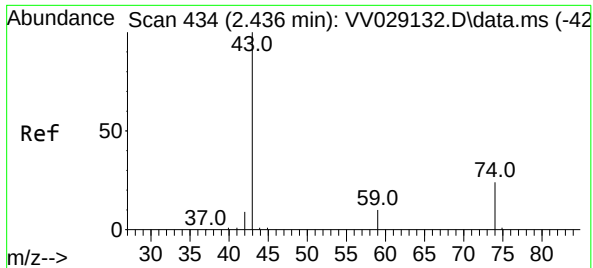

#15
Methyl Acetate
Concen: 0.759 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.013 min
Lab File: VV029153.D
Acq: 19 Nov 2022 06:06

Instrument :
MSVOA_V
ClientSampleId :
BHB29

Tgt Ion: 43 Resp: 3582
Ion Ratio Lower Upper
43 100
74 13.6 24.6 37.0#

