

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029112.D
 Acq On : 18 Nov 2022 12:46
 Operator : SY/MD
 Sample : N5687-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	73	rVV4	8854	13415	1.45%	0.179%
2	1.304	76	82	93	rVV	116378	119105	12.89%	1.593%
3	1.468	119	133	136	rBV2	31412	65804	7.12%	0.880%
4	1.564	157	163	177	rVB	107327	127770	13.83%	1.709%
5	2.105	322	331	349	rVB	229050	350037	37.89%	4.682%
6	2.764	528	536	548	rVB7	5081	9749	1.06%	0.130%
7	3.912	882	893	909	rBV	45775	163554	17.70%	2.188%
8	4.346	1012	1028	1065	rVB2	152418	395768	42.84%	5.294%
9	5.043	1229	1245	1276	rBV2	360246	923798	100.00%	12.357%
10	5.616	1411	1423	1451	rBV	284205	595798	64.49%	7.970%
11	5.921	1507	1518	1535	rBV5	9618	20940	2.27%	0.280%
12	6.066	1550	1563	1593	rBV	205009	445205	48.19%	5.955%
13	6.985	1835	1849	1870	rBV	90186	178221	19.29%	2.384%
14	7.313	1939	1951	1972	rBV	430717	769088	83.25%	10.288%
15	7.622	2037	2047	2065	rBV2	47397	92788	10.04%	1.241%
16	8.091	2181	2193	2238	rBV2	347662	876790	94.91%	11.728%
17	8.847	2415	2428	2451	rBV	409941	699118	75.68%	9.352%
18	10.210	2838	2852	2878	rBV	153517	259306	28.07%	3.469%
19	11.242	3162	3173	3197	rVV	403262	656667	71.08%	8.784%
20	11.615	3277	3289	3316	rBV	404056	678765	73.48%	9.080%
21	15.879	4600	4615	4618	rBV	14749	34038	3.68%	0.455%




Sum of corrected areas: 7475724

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029112.D
Acq On : 18 Nov 2022 12:46
Operator : SY/MD
Sample : N5687-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

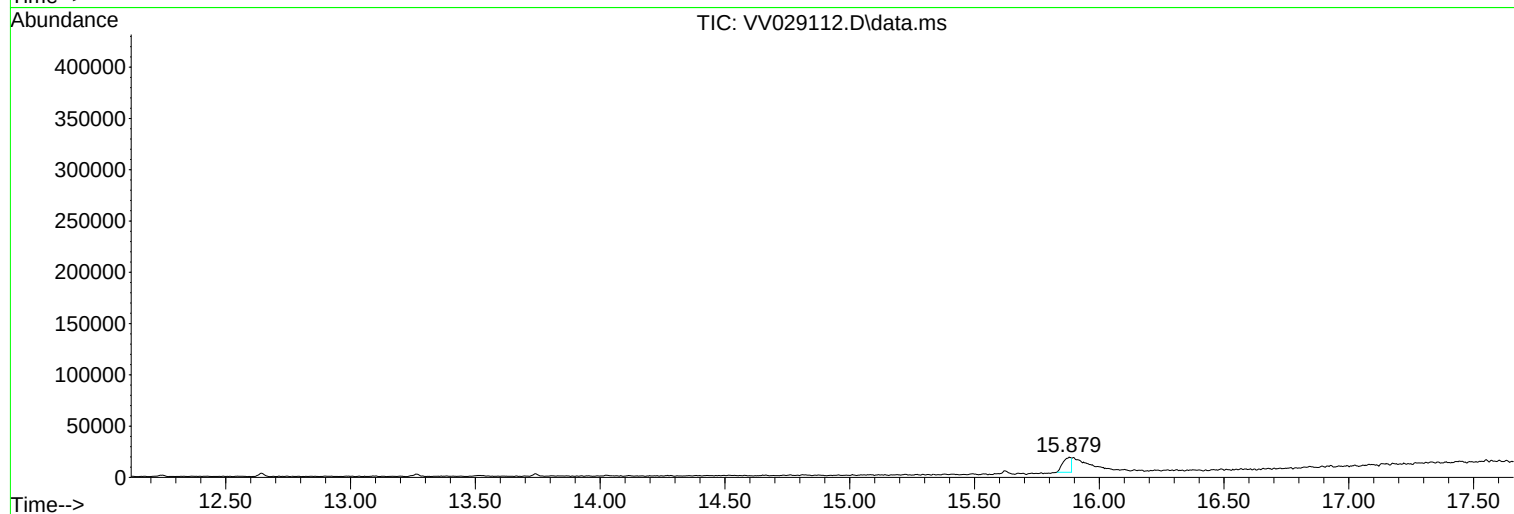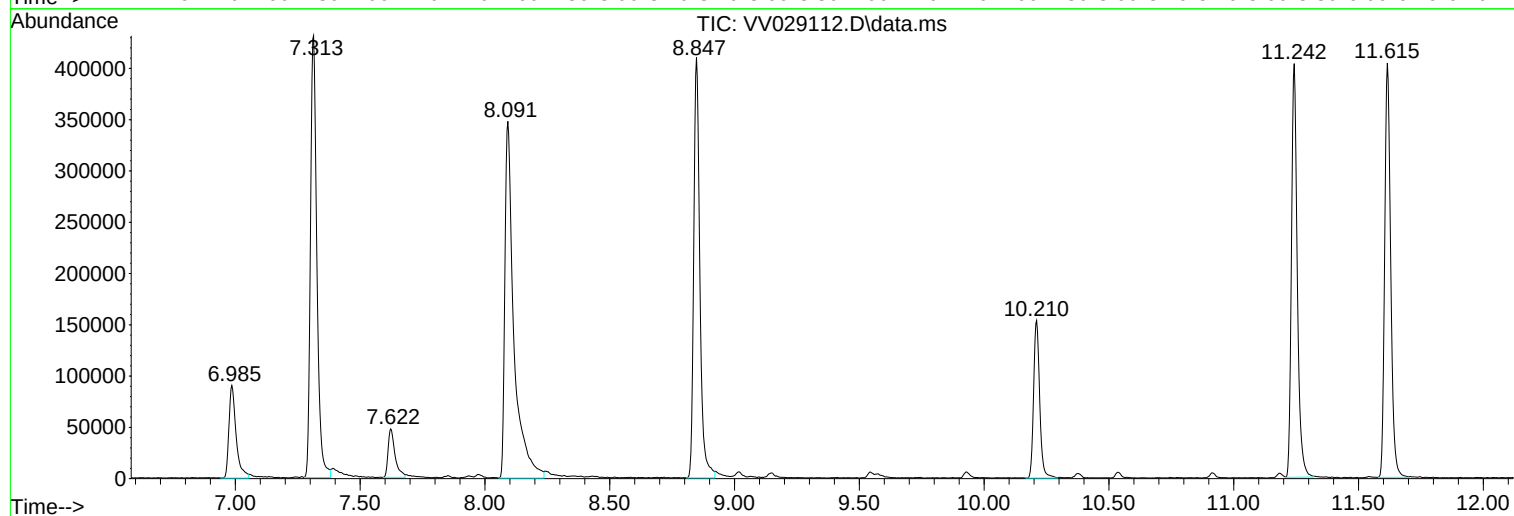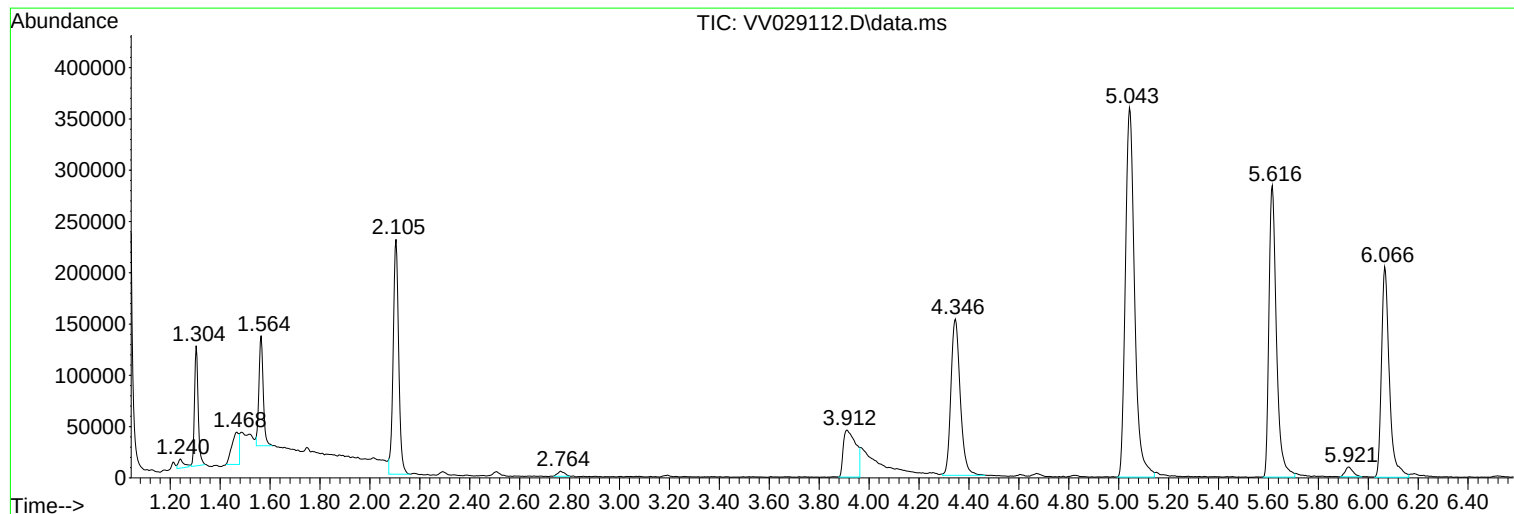

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029112.D
Acq On : 18 Nov 2022 12:46
Operator : SY/MD
Sample : N5687-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029112.D
Acq On : 18 Nov 2022 12:46
Operator : SY/MD
Sample : N5687-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc