

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029115.D
 Acq On : 18 Nov 2022 13:57
 Operator : SY/MD
 Sample : N5687-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCD5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	57	63	74	rBV2	18988	34820	1.35%	0.291%
2	1.307	76	83	100	rVB	112828	130556	5.06%	1.093%
3	1.420	105	118	147	rBV2	61382	323633	12.55%	2.708%
4	1.568	158	164	183	rVB	110184	135572	5.26%	1.135%
5	2.108	322	332	347	rVB	222298	337465	13.09%	2.824%
6	3.191	654	669	692	rVB	36929	77654	3.01%	0.650%
7	3.908	876	892	933	rBV2	494925	1354243	52.52%	11.333%
8	4.346	1013	1028	1050	rVB	157227	391145	15.17%	3.273%
9	4.606	1093	1109	1128	rBV2	44619	113196	4.39%	0.947%
10	5.046	1231	1246	1288	rBV2	368881	965256	37.44%	8.078%
11	5.616	1409	1423	1454	rBV	305933	655019	25.40%	5.482%
12	5.911	1501	1515	1548	rBV	1300058	2578369	100.00%	21.578%
13	6.069	1551	1564	1594	rVB	210052	452138	17.54%	3.784%
14	6.985	1838	1849	1874	rBV	91123	182705	7.09%	1.529%
15	7.313	1940	1951	1997	rBV	444060	822232	31.89%	6.881%
16	7.622	2038	2047	2069	rBV	49637	99912	3.88%	0.836%
17	8.091	2182	2193	2244	rBV2	294359	901351	34.96%	7.543%
18	8.847	2416	2428	2457	rBV	452069	765796	29.70%	6.409%
19	10.210	2840	2852	2877	rBV	159051	263451	10.22%	2.205%
20	10.377	2893	2904	2918	rBV	19392	31762	1.23%	0.266%
21	11.242	3162	3173	3196	rBV	406922	667840	25.90%	5.589%
22	11.615	3277	3289	3312	rBV	405610	665043	25.79%	5.566%




Sum of corrected areas: 11949158

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029115.D
Acq On : 18 Nov 2022 13:57
Operator : SY/MD
Sample : N5687-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

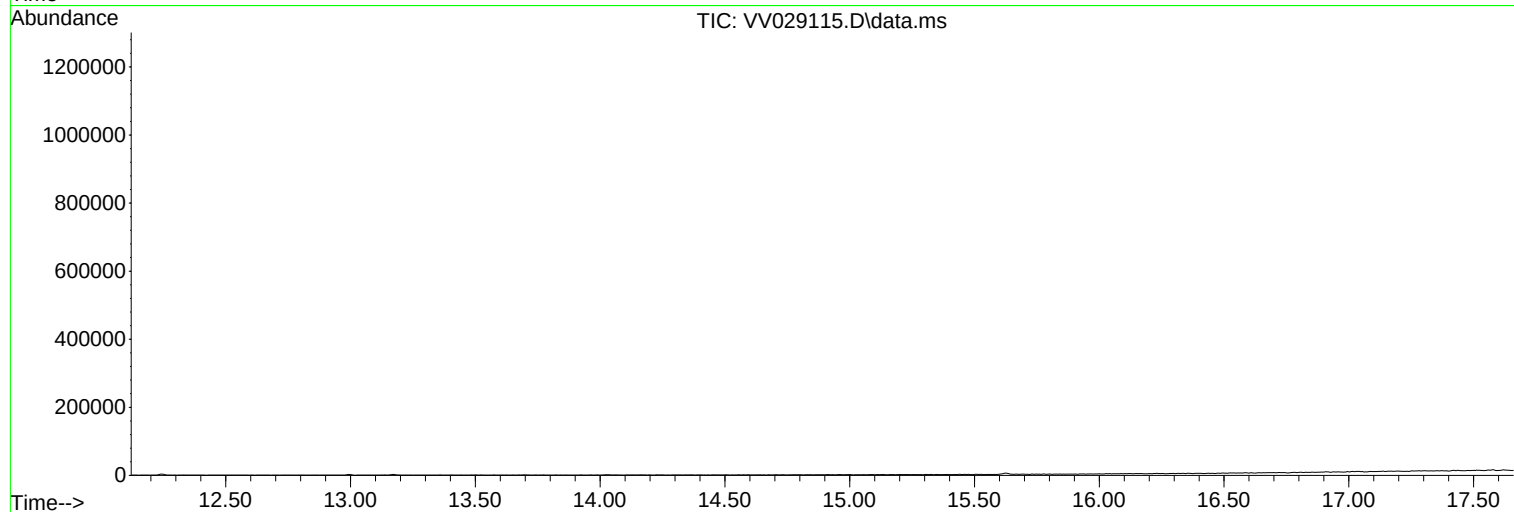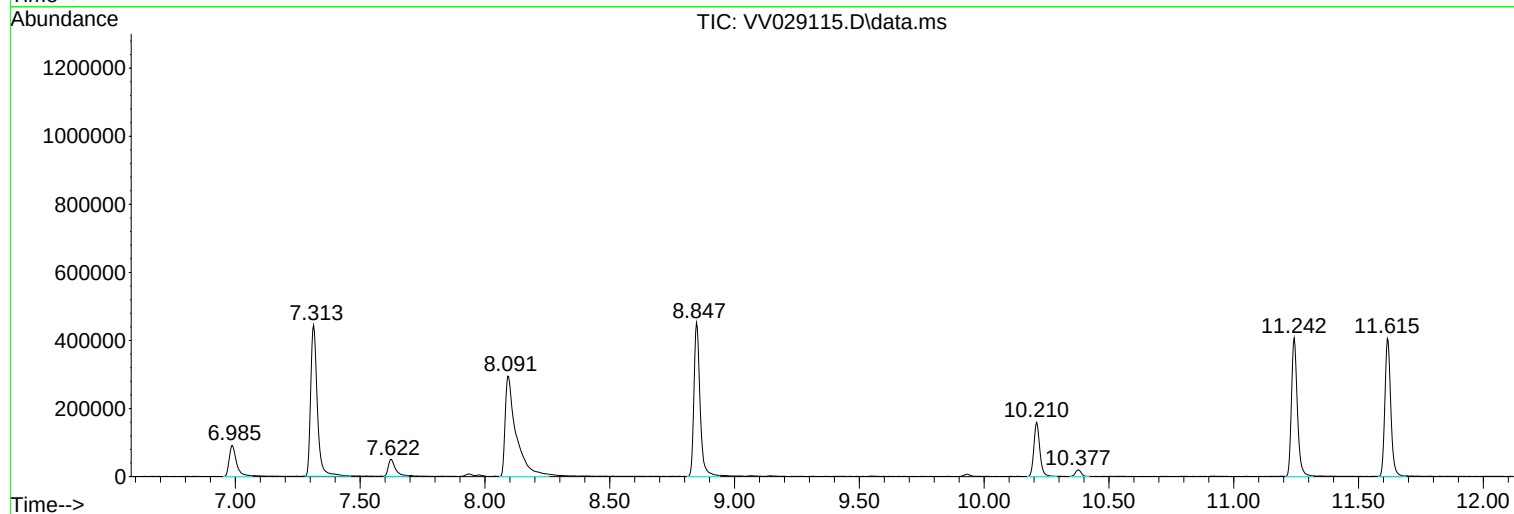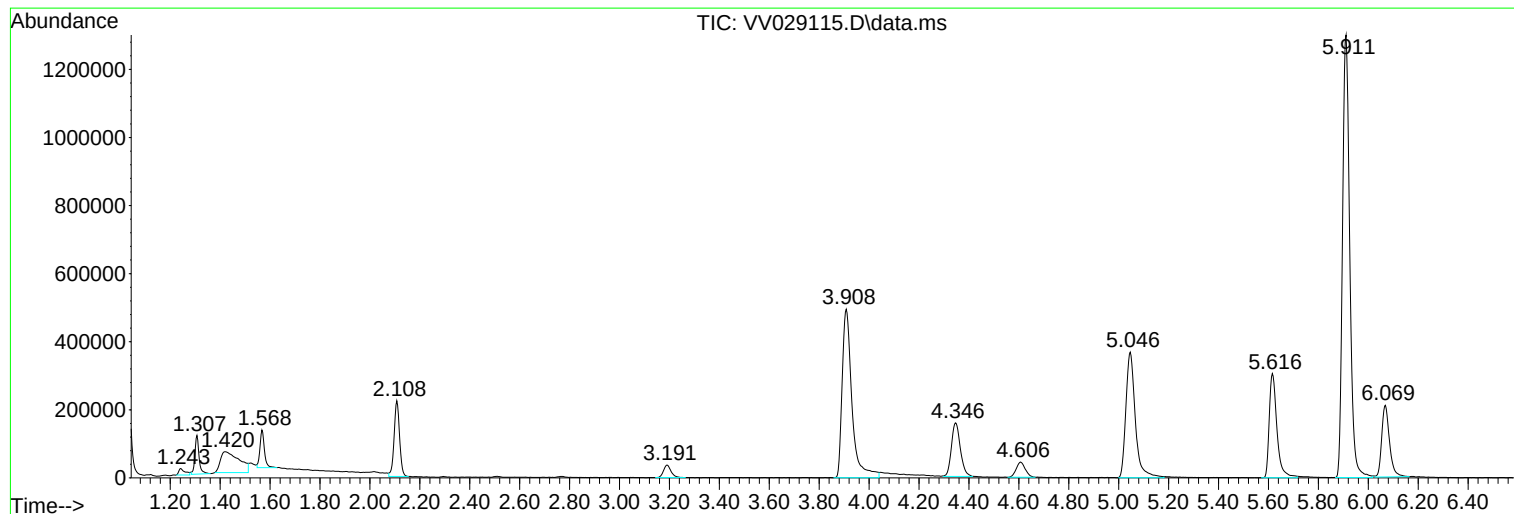

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029115.D
Acq On : 18 Nov 2022 13:57
Operator : SY/MD
Sample : N5687-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.420	2.5	ug/L	323633	1	5.616	655019	5.0