

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029121.D
 Acq On : 18 Nov 2022 16:24
 Operator : SY/MD
 Sample : N5687-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	56	63	65	rBV	9132	9724	1.06%	0.131%
2	1.307	76	83	100	rVB	107465	119616	13.02%	1.609%
3	1.426	109	120	122	rBV	31092	48481	5.28%	0.652%
4	1.568	157	164	181	rVB	107444	130218	14.17%	1.751%
5	2.015	297	303	313	rVB2	12726	18608	2.02%	0.250%
6	2.108	322	332	348	rVB	212153	320872	34.91%	4.316%
7	3.905	879	891	927	rBV2	45483	201167	21.89%	2.706%
8	4.342	1013	1027	1057	rVB2	154483	401160	43.65%	5.395%
9	5.043	1228	1245	1277	rBV3	359605	919016	100.00%	12.360%
10	5.612	1410	1422	1454	rBV	289017	602691	65.58%	8.106%
11	6.066	1549	1563	1587	rBV	205143	436427	47.49%	5.870%
12	6.985	1835	1849	1869	rBV	90634	178259	19.40%	2.397%
13	7.313	1939	1951	1975	rBV	435621	794545	86.46%	10.686%
14	7.622	2037	2047	2068	rBV	49173	94792	10.31%	1.275%
15	7.934	2130	2144	2153	rBV3	7219	13002	1.41%	0.175%
16	8.091	2183	2193	2252	rBV2	259670	873761	95.08%	11.752%
17	8.847	2417	2428	2457	rBV	414415	712200	77.50%	9.579%
18	10.210	2840	2852	2873	rBV	150503	256957	27.96%	3.456%
19	10.378	2893	2904	2919	rVB	20099	33693	3.67%	0.453%
20	11.242	3161	3173	3199	rBV	379626	623904	67.89%	8.391%
21	11.615	3275	3289	3312	rBV	382885	646164	70.31%	8.691%




Sum of corrected areas: 7435257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029121.D
Acq On : 18 Nov 2022 16:24
Operator : SY/MD
Sample : N5687-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

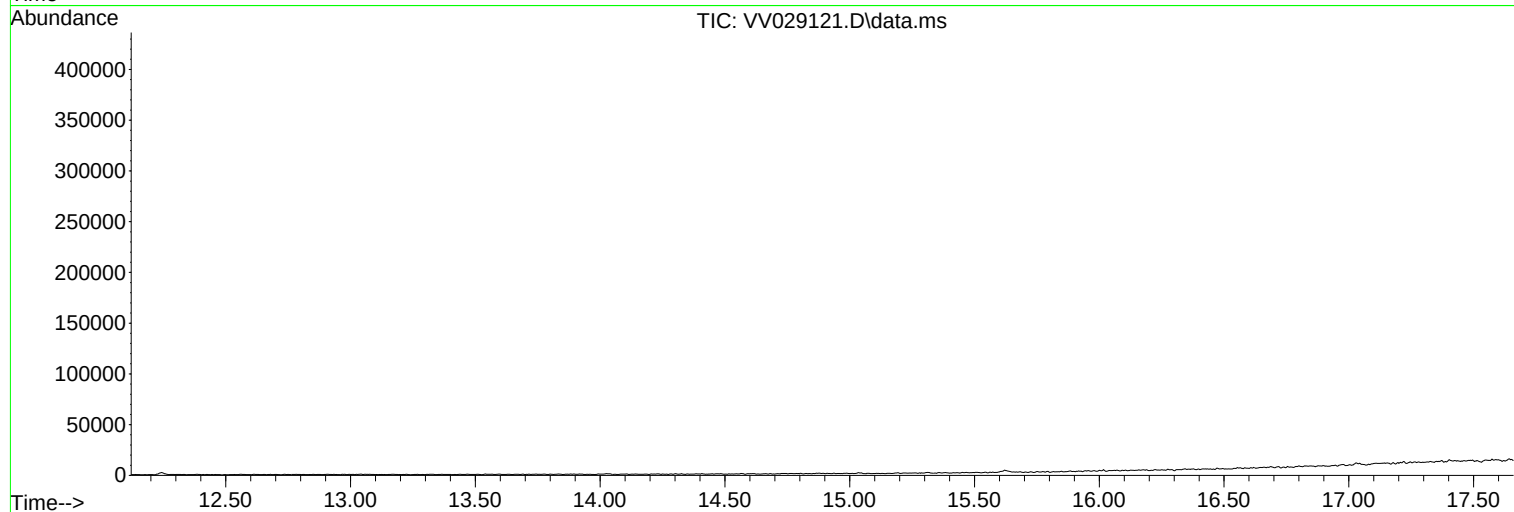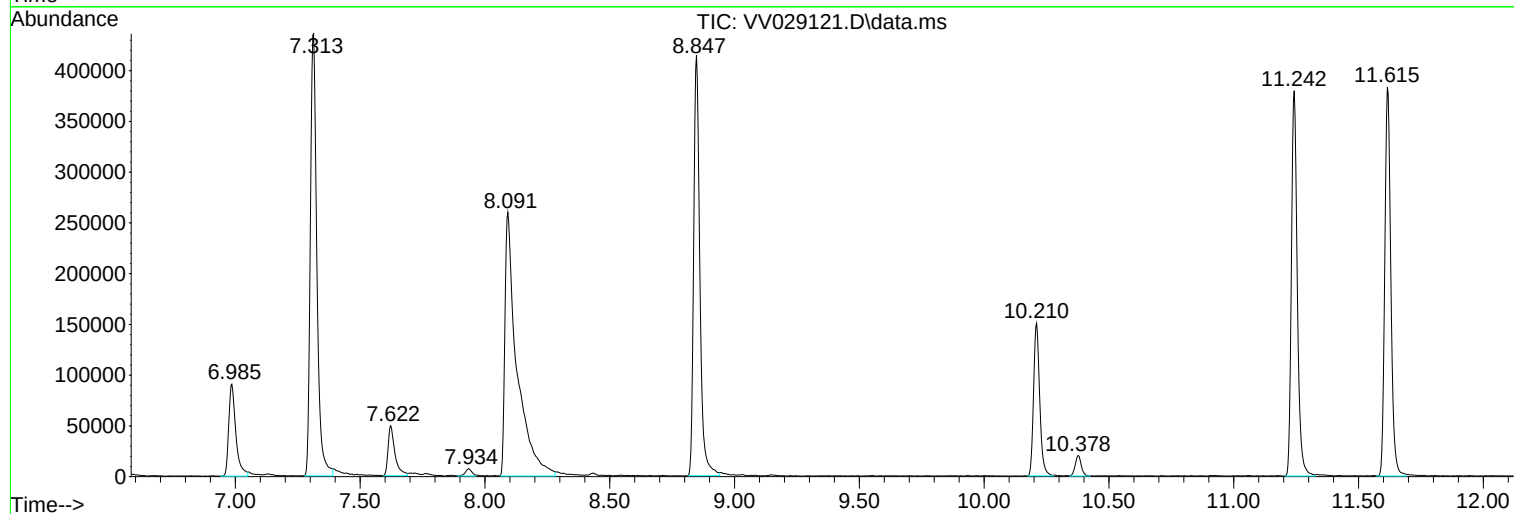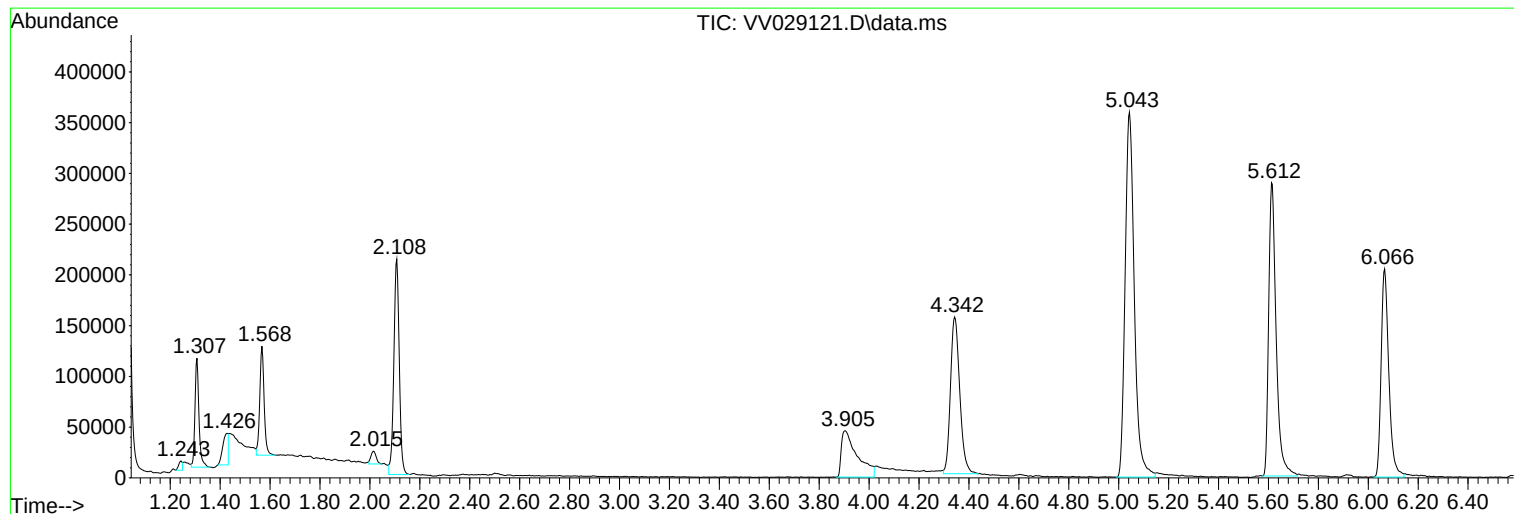

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029121.D
Acq On : 18 Nov 2022 16:24
Operator : SY/MD
Sample : N5687-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029121.D
Acq On : 18 Nov 2022 16:24
Operator : SY/MD
Sample : N5687-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc