

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029131.D
 Acq On : 18 Nov 2022 20:27
 Operator : SY/MD
 Sample : N5688-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCF4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	36	44	54	rBV	14958	32322	3.38%	0.419%
2	1.298	74	80	99	rVB	110613	120825	12.65%	1.568%
3	1.558	153	161	174	rBV	108111	122229	12.80%	1.586%
4	1.931	268	277	286	rBV2	18253	44541	4.66%	0.578%
5	2.095	320	328	356	rVB	216144	339441	35.54%	4.405%
6	3.960	889	908	940	rBV2	59693	276309	28.93%	3.586%
7	4.333	1007	1024	1044	rVB	166728	405534	42.46%	5.263%
8	5.031	1224	1241	1265	rBV2	429554	955094	100.00%	12.394%
9	5.603	1405	1419	1443	rVB	339807	671491	70.31%	8.714%
10	6.063	1549	1562	1583	rBV	234230	471564	49.37%	6.119%
11	6.725	1763	1768	1786	rBV	15324	36351	3.81%	0.472%
12	6.979	1836	1847	1866	rBV2	82809	148602	15.56%	1.928%
13	7.307	1935	1949	1967	rBV	452084	789806	82.69%	10.249%
14	7.619	2036	2046	2068	rBV	43233	78548	8.22%	1.019%
15	8.104	2186	2197	2242	rBV2	386552	891559	93.35%	11.570%
16	8.844	2413	2427	2457	rBV	442185	728292	76.25%	9.451%
17	10.210	2840	2852	2874	rBV	165063	260086	27.23%	3.375%
18	10.374	2893	2903	2913	rBV3	12361	20058	2.10%	0.260%
19	11.239	3161	3172	3196	rBV	404009	634603	66.44%	8.235%
20	11.616	3277	3289	3310	rBV	398479	651466	68.21%	8.454%
21	15.882	4599	4616	4617	rBV10	12768	27231	2.85%	0.353%




Sum of corrected areas: 7705952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029131.D
Acq On : 18 Nov 2022 20:27
Operator : SY/MD
Sample : N5688-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

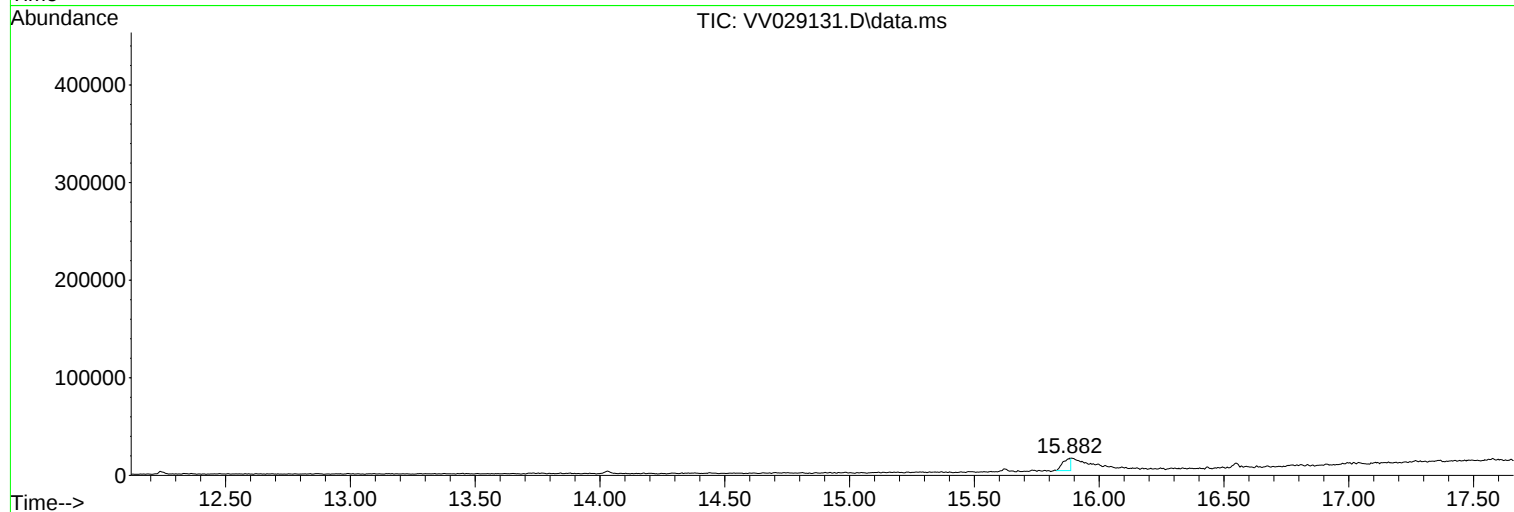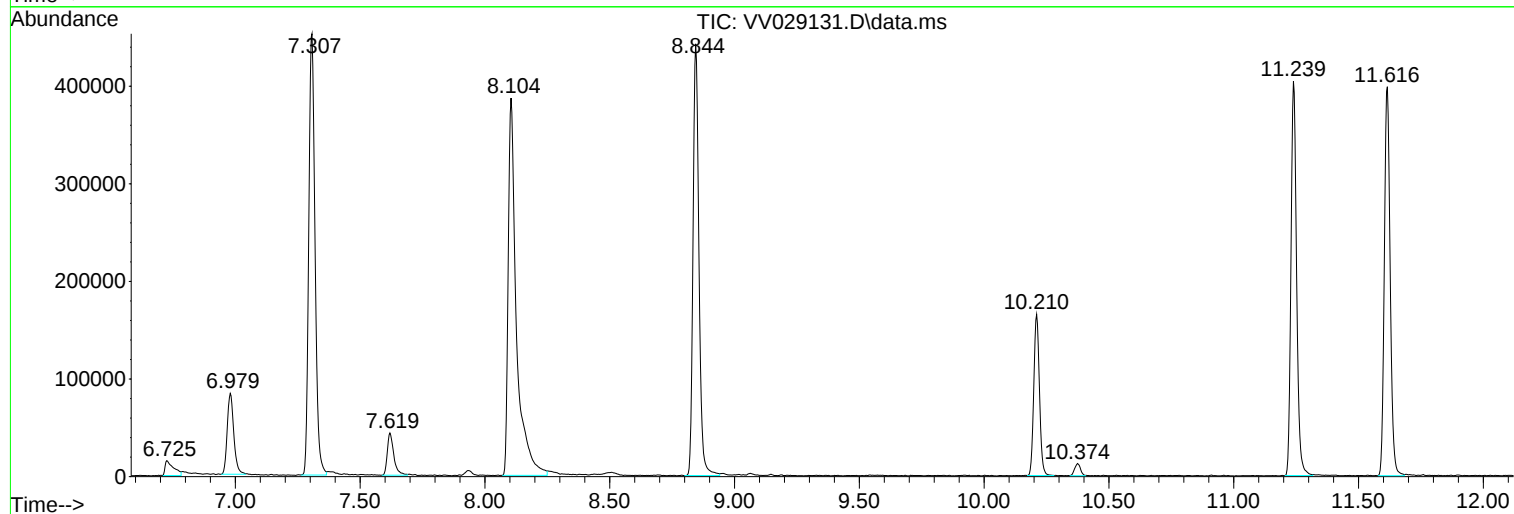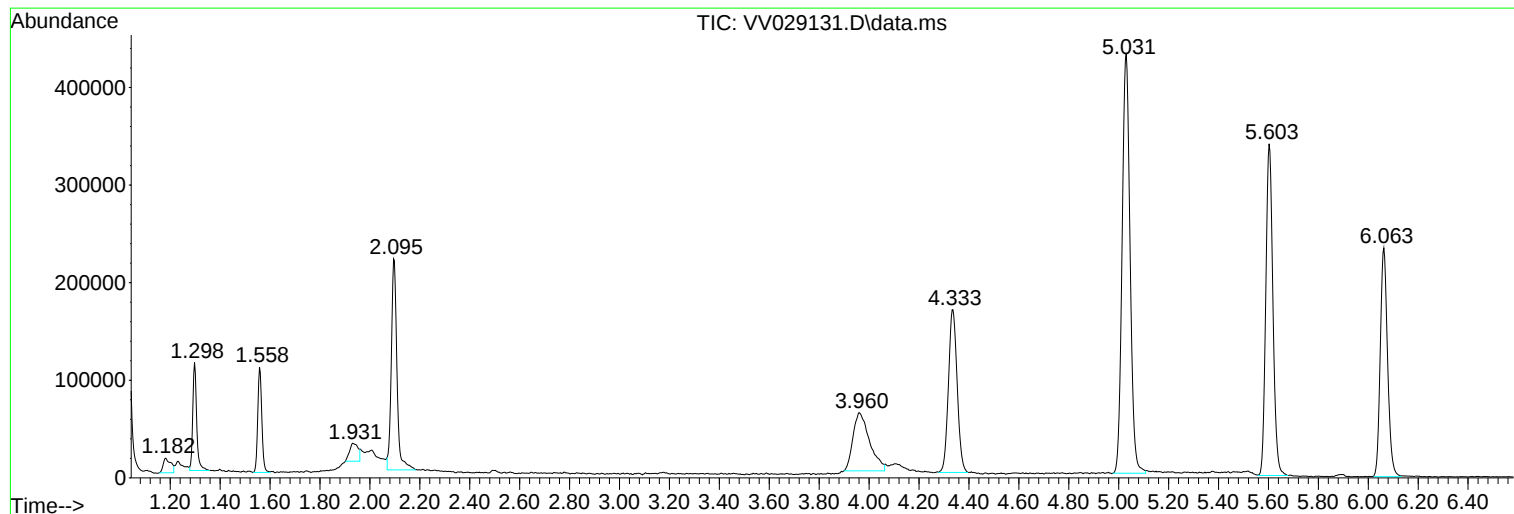

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029131.D
Acq On : 18 Nov 2022 20:27
Operator : SY/MD
Sample : N5688-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.979	1.11 ug/L	148602	1,4-Difluorobenzene	5.603

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	38
2			1,3-Cyclohexadiene	80	C6H8	000592-57-4	28
3			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	28
4			1,3-Cyclohexadiene	80	C6H8	000592-57-4	28
5			3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	9

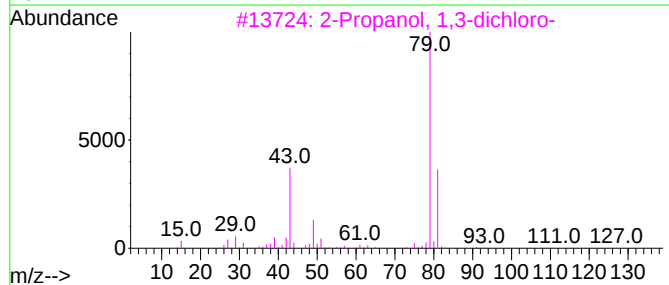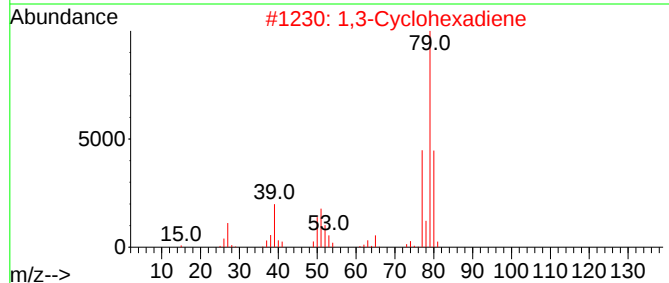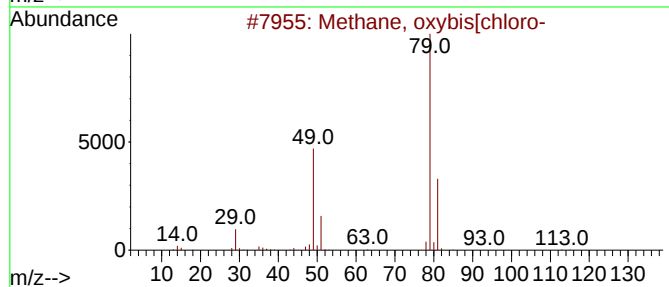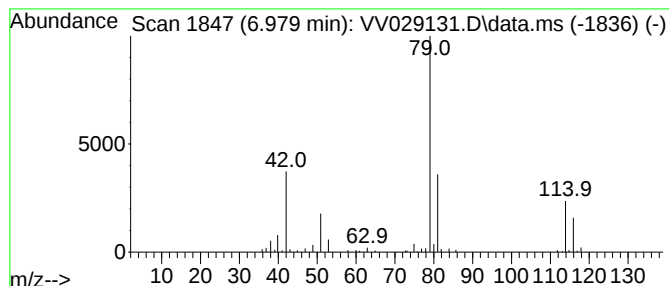

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029131.D
Acq On : 18 Nov 2022 20:27
Operator : SY/MD
Sample : N5688-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	6.979	1.1	ug/L	148602	1	5.603	671491	5.0