

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029134.D
 Acq On : 18 Nov 2022 22:22
 Operator : SY/MD
 Sample : N5688-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCF5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	105177	113012	9.43%	1.265%
2	1.478	117	136	138	rBV	27009	55195	4.61%	0.618%
3	1.568	158	164	181	rVB	105300	125840	10.50%	1.409%
4	2.015	296	303	316	rVB	25676	38058	3.18%	0.426%
5	2.108	322	332	347	rVB	194929	292186	24.39%	3.271%
6	3.905	877	891	921	rBV3	174543	589950	49.24%	6.604%
7	4.342	1012	1027	1061	rVB	152959	394789	32.95%	4.419%
8	4.606	1095	1109	1123	rBV4	12454	30318	2.53%	0.339%
9	5.043	1229	1245	1282	rBV2	349349	907259	75.73%	10.156%
10	5.613	1410	1422	1464	rBV	294232	624847	52.15%	6.995%
11	5.908	1496	1514	1547	rBV	596777	1198096	100.00%	13.412%
12	6.066	1551	1563	1588	rVV	204524	427425	35.68%	4.785%
13	6.982	1836	1848	1874	rBV	87316	175628	14.66%	1.966%
14	7.310	1938	1950	1977	rBV	414418	755748	63.08%	8.460%
15	7.622	2037	2047	2069	rBV2	47176	94376	7.88%	1.056%
16	8.088	2181	2192	2239	rBV3	342926	880434	73.49%	9.856%
17	8.847	2415	2428	2460	rBV	425167	726150	60.61%	8.129%
18	10.210	2839	2852	2871	rBV	150158	245045	20.45%	2.743%
19	11.239	3161	3172	3205	rBV	383956	632030	52.75%	7.075%
20	11.615	3277	3289	3313	rBV	390031	626575	52.30%	7.014%




Sum of corrected areas: 8932961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029134.D
Acq On : 18 Nov 2022 22:22
Operator : SY/MD
Sample : N5688-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

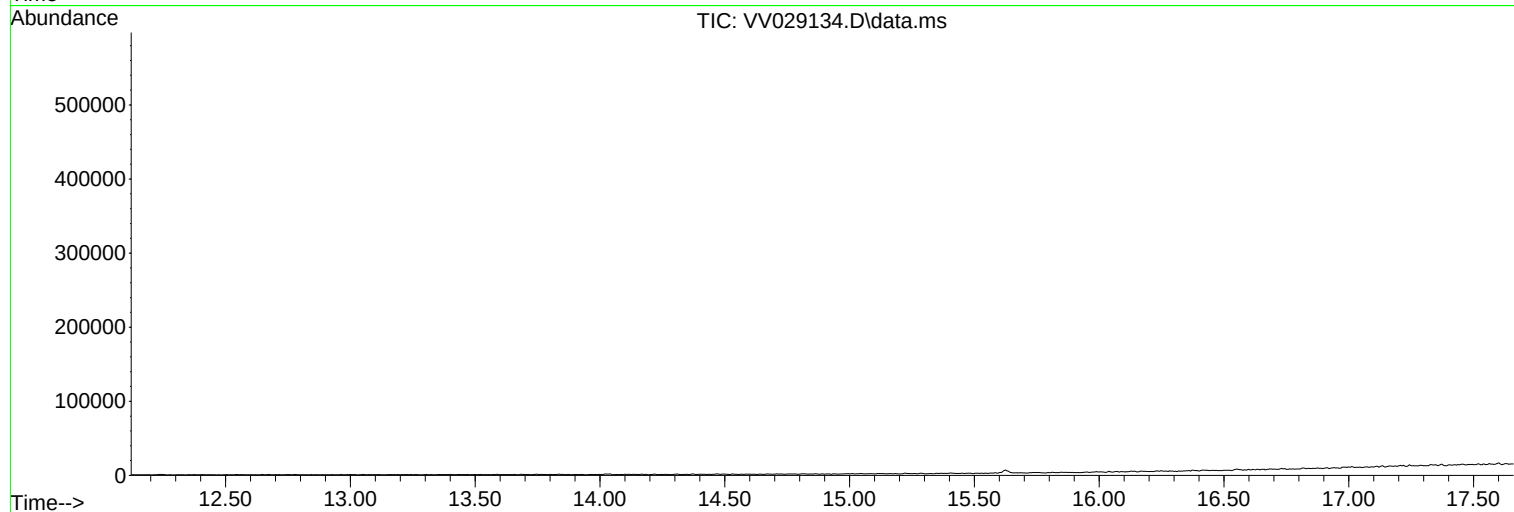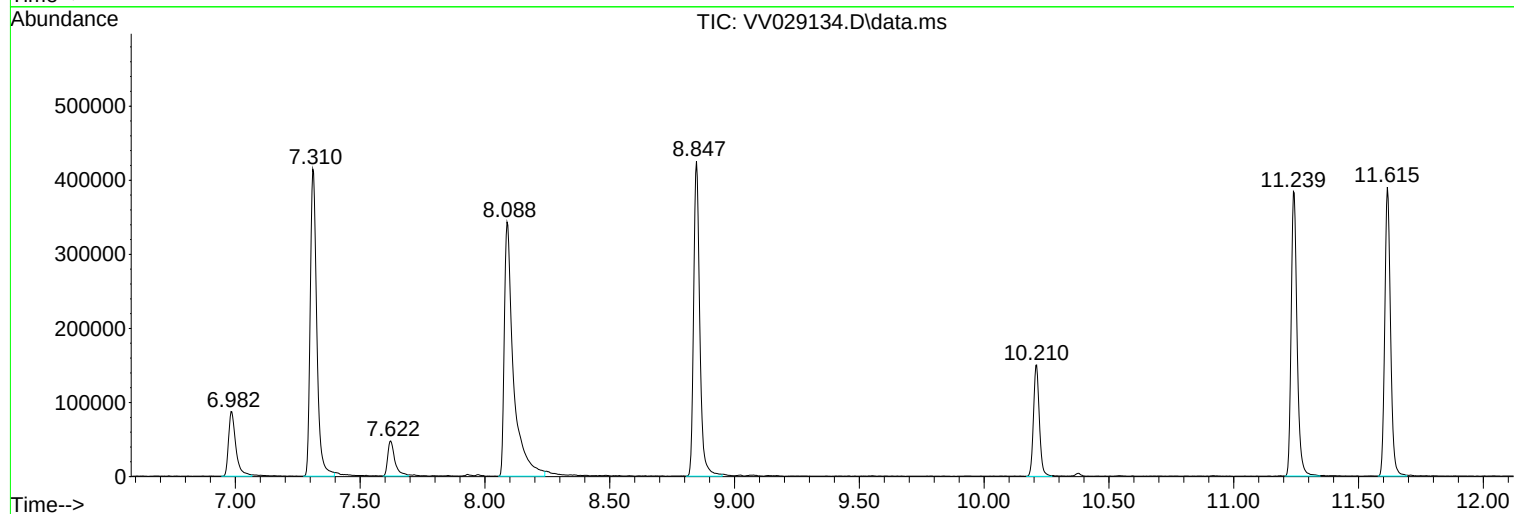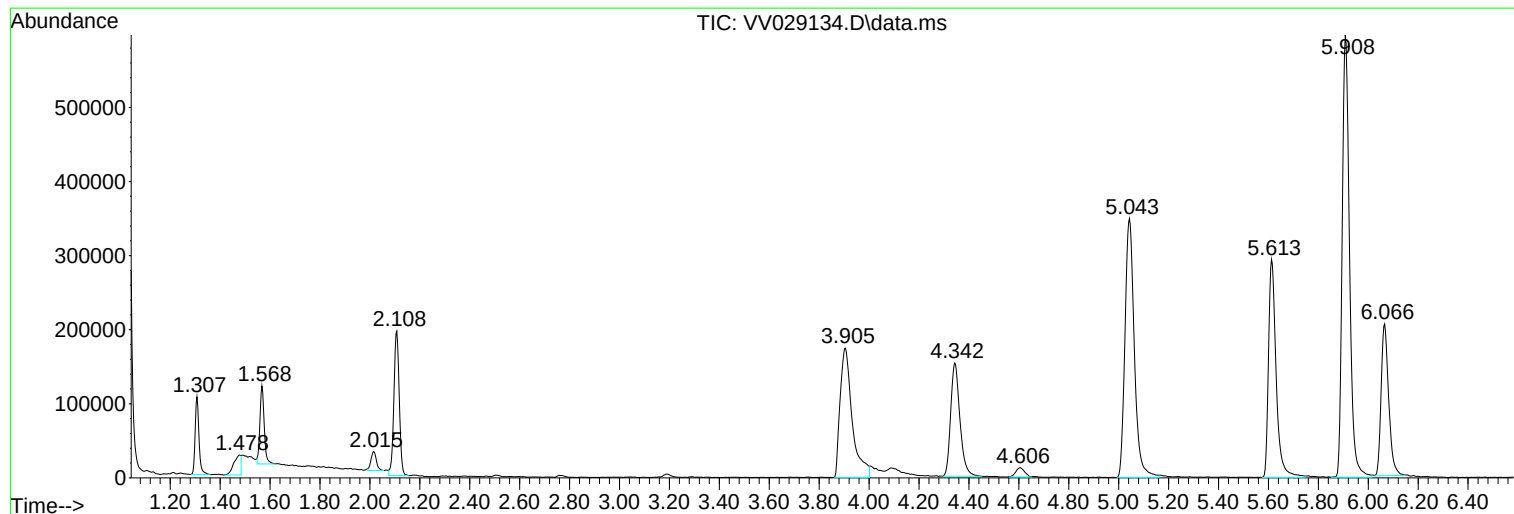

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029134.D
Acq On : 18 Nov 2022 22:22
Operator : SY/MD
Sample : N5688-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029134.D
Acq On : 18 Nov 2022 22:22
Operator : SY/MD
Sample : N5688-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc