

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029135.D
 Acq On : 18 Nov 2022 22:46
 Operator : SY/MD
 Sample : N5688-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCF6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	96094	106235	11.88%	1.423%
2	1.568	156	164	176	rBV	97080	112213	12.55%	1.503%
3	2.105	322	331	349	rVB	198630	294047	32.89%	3.939%
4	3.185	656	667	684	rBV	12224	25730	2.88%	0.345%
5	3.909	875	892	929	rBV2	162430	515768	57.69%	6.909%
6	4.092	942	949	968	rVB5	10206	26482	2.96%	0.355%
7	4.343	1013	1027	1056	rVB3	150606	405903	45.40%	5.437%
8	5.044	1228	1245	1277	rBV2	342589	869678	97.28%	11.650%
9	5.613	1411	1422	1458	rBV	287025	602842	67.43%	8.076%
10	6.066	1549	1563	1586	rBV	197962	419542	46.93%	5.620%
11	6.986	1838	1849	1869	rBV	83757	164412	18.39%	2.202%
12	7.310	1939	1950	1971	rBV	399885	717573	80.27%	9.612%
13	7.622	2037	2047	2078	rBV	48103	95109	10.64%	1.274%
14	8.088	2182	2192	2250	rBV2	295857	893986	100.00%	11.976%
15	8.847	2413	2428	2460	rBV	417603	708974	79.30%	9.497%
16	10.211	2840	2852	2872	rBV	151809	254605	28.48%	3.411%
17	10.374	2893	2903	2915	rVB3	8075	13783	1.54%	0.185%
18	11.239	3161	3172	3197	rBV	380012	619872	69.34%	8.304%
19	11.616	3276	3289	3314	rBV	380826	618286	69.16%	8.282%




Sum of corrected areas: 7465040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029135.D
Acq On : 18 Nov 2022 22:46
Operator : SY/MD
Sample : N5688-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

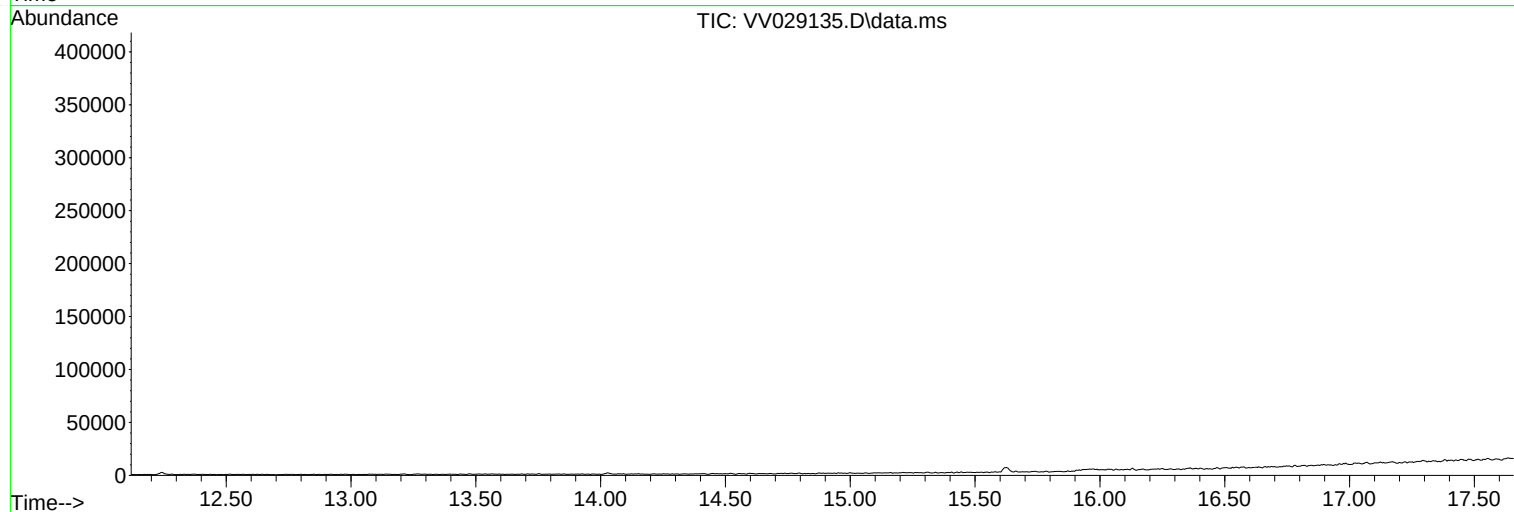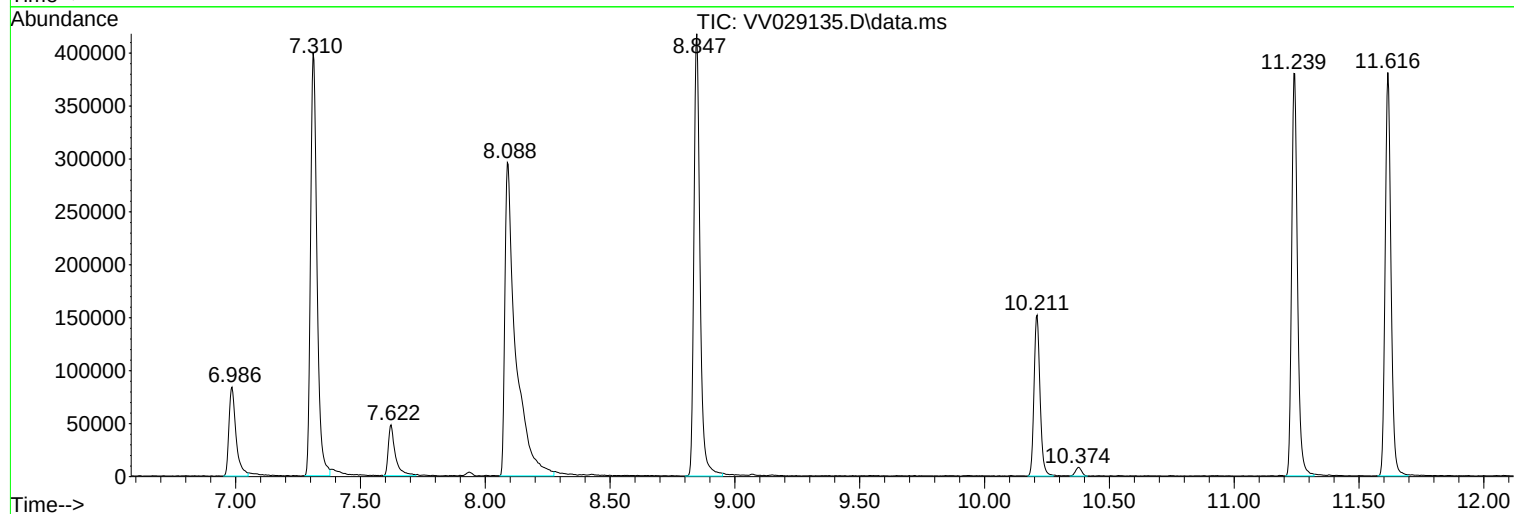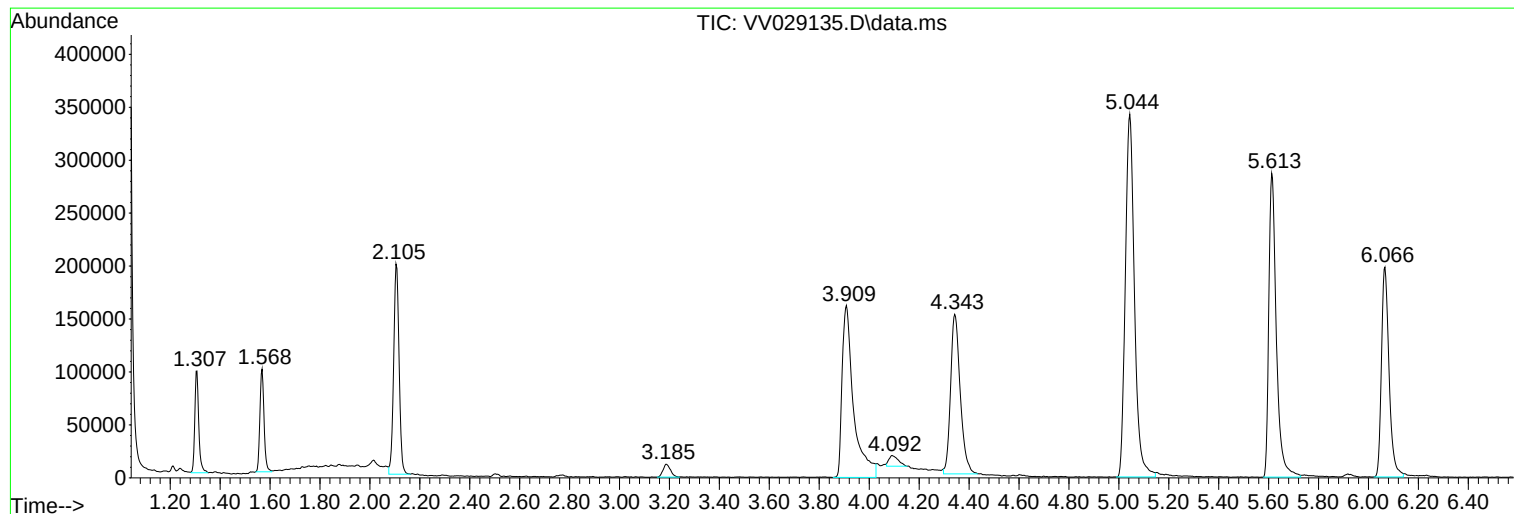

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029135.D
Acq On : 18 Nov 2022 22:46
Operator : SY/MD
Sample : N5688-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029135.D
Acq On : 18 Nov 2022 22:46
Operator : SY/MD
Sample : N5688-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc