

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029137.D
 Acq On : 18 Nov 2022 23:35
 Operator : SY/MD
 Sample : N5688-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	101842	107116	6.38%	1.185%
2	1.523	130	150	153	rBV3	12840	30495	1.82%	0.337%
3	1.568	157	164	181	rVB	105575	134238	7.99%	1.485%
4	2.108	322	332	355	rVB	205434	318402	18.95%	3.523%
5	3.188	654	668	685	rBV	20087	43623	2.60%	0.483%
6	3.905	876	891	932	rBV2	630322	1680145	100.00%	18.589%
7	4.342	1011	1027	1056	rBV	153891	396385	23.59%	4.386%
8	4.606	1091	1109	1129	rVB3	49810	129445	7.70%	1.432%
9	5.043	1228	1245	1276	rBV2	353381	909883	54.16%	10.067%
10	5.612	1409	1422	1451	rBV	286241	611920	36.42%	6.770%
11	6.066	1549	1563	1600	rBV	206265	439010	26.13%	4.857%
12	6.985	1836	1849	1876	rBV2	89995	180862	10.76%	2.001%
13	7.313	1938	1951	1989	rBV	417858	773146	46.02%	8.554%
14	7.622	2035	2047	2069	rBV2	49416	96206	5.73%	1.064%
15	8.091	2181	2193	2250	rBV2	312907	883449	52.58%	9.774%
16	8.847	2413	2428	2463	rBV	427581	722898	43.03%	7.998%
17	10.210	2839	2852	2872	rBV	156811	262064	15.60%	2.899%
18	10.377	2892	2904	2916	rBV2	15965	26796	1.59%	0.296%
19	11.242	3161	3173	3201	rBV	389698	642987	38.27%	7.114%
20	11.615	3275	3289	3316	rBV	394202	649321	38.65%	7.184%




Sum of corrected areas: 9038391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029137.D
Acq On : 18 Nov 2022 23:35
Operator : SY/MD
Sample : N5688-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

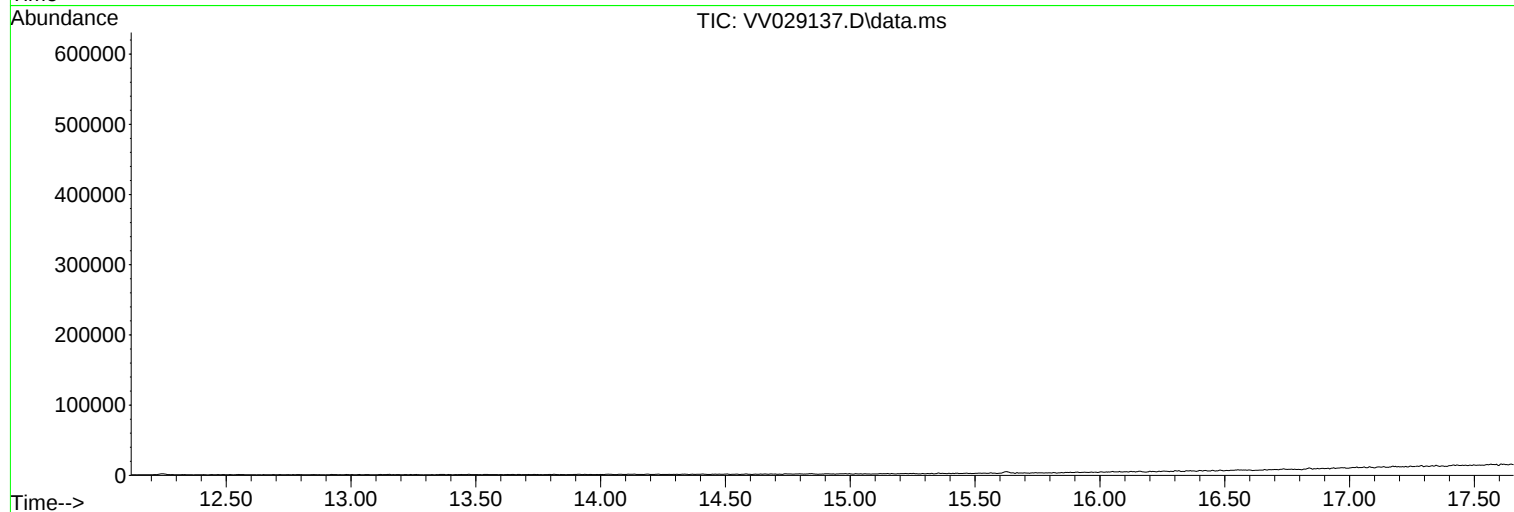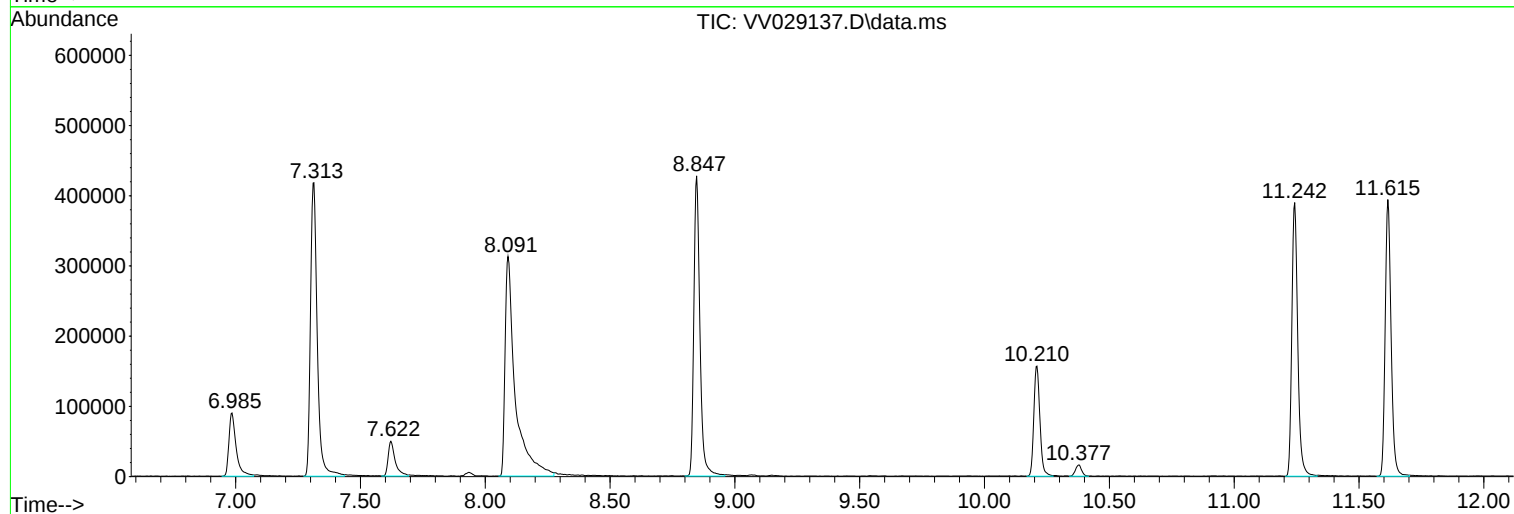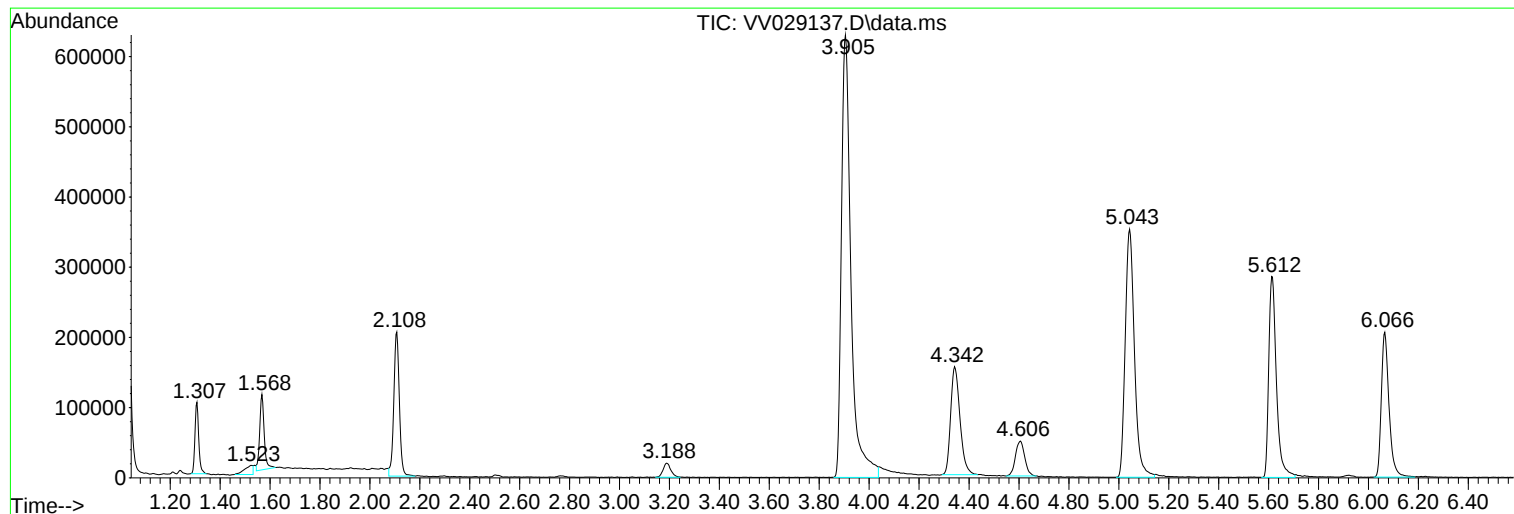

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029137.D
Acq On : 18 Nov 2022 23:35
Operator : SY/MD
Sample : N5688-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.985	1.48 ug/L	180862	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	38		
2	2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	28		
3	1,3-Cyclohexadiene	80	C6H8	000592-57-4	28		
4	Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	28		
5	2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	28		

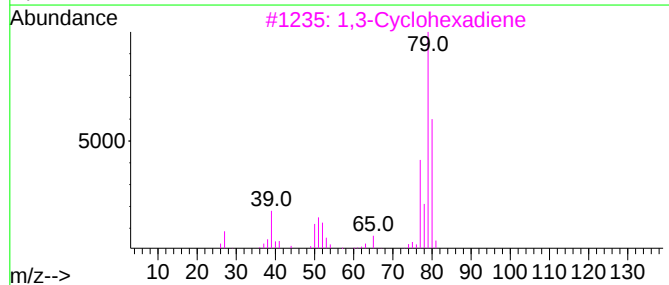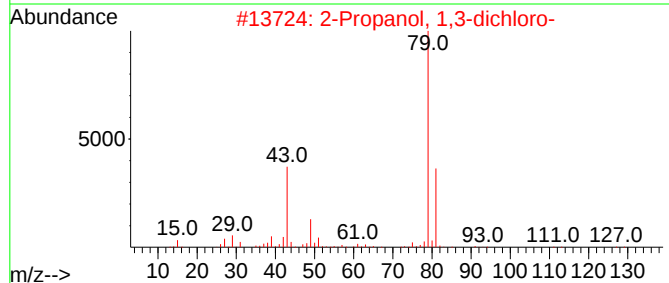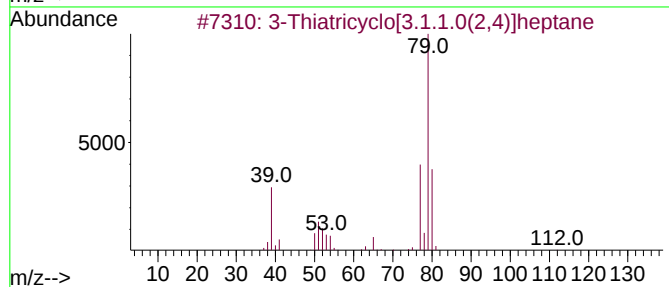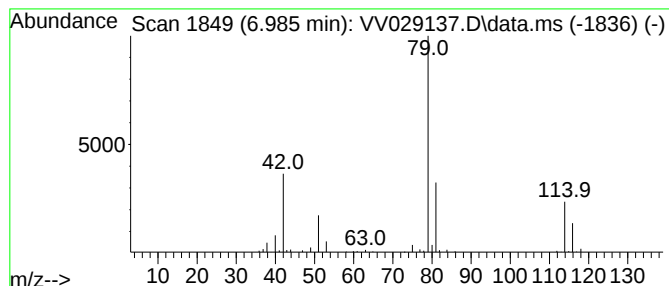

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029137.D
Acq On : 18 Nov 2022 23:35
Operator : SY/MD
Sample : N5688-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	6.985	1.5	ug/L	180862	1	5.616	611920	5.0