

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029141.D
 Acq On : 19 Nov 2022 01:13
 Operator : SY/MD
 Sample : N5688-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	74	rBV	8591	9923	1.12%	0.137%
2	1.307	75	83	94	rBV	100420	104833	11.86%	1.446%
3	1.568	156	164	172	rBV	100493	122359	13.84%	1.688%
4	2.105	322	331	350	rVB	190167	284548	32.19%	3.926%
5	3.918	885	895	942	rBV2	51756	283953	32.12%	3.917%
6	4.342	1012	1027	1049	rBV	151160	377534	42.71%	5.209%
7	5.043	1224	1245	1281	rBV2	345192	884000	100.00%	12.196%
8	5.612	1411	1422	1445	rBV	289274	600205	67.90%	8.281%
9	6.066	1544	1563	1588	rBV	197974	422225	47.76%	5.825%
10	6.985	1838	1849	1873	rBV2	85004	173112	19.58%	2.388%
11	7.313	1939	1951	1974	rBV	411523	739757	83.68%	10.206%
12	7.622	2035	2047	2069	rBV2	46869	93682	10.60%	1.292%
13	7.934	2134	2144	2157	rVB2	7503	13640	1.54%	0.188%
14	8.091	2183	2193	2232	rBV2	354490	880800	99.64%	12.152%
15	8.847	2416	2428	2452	rBV	424228	713744	80.74%	9.847%
16	10.210	2841	2852	2875	rBV2	160014	261058	29.53%	3.602%
17	10.374	2892	2903	2915	rBV3	20957	34660	3.92%	0.478%
18	11.242	3162	3173	3196	rBV	380240	617244	69.82%	8.516%
19	11.615	3277	3289	3308	rBV	383370	631095	71.39%	8.707%




Sum of corrected areas: 7248372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029141.D
Acq On : 19 Nov 2022 01:13
Operator : SY/MD
Sample : N5688-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

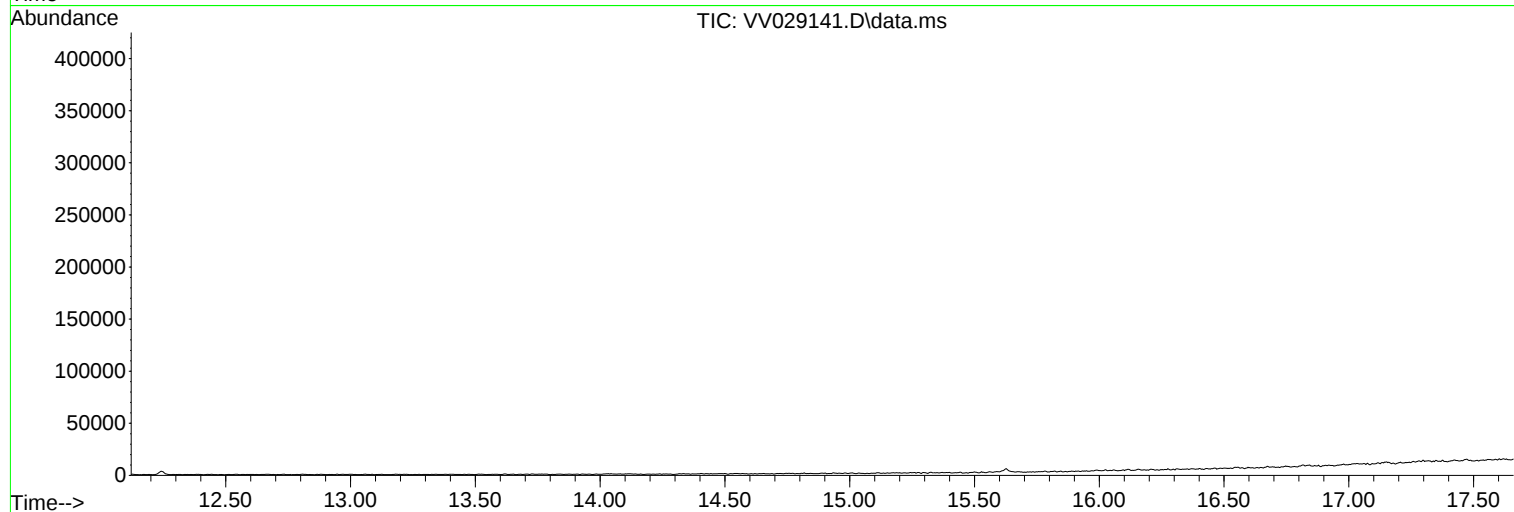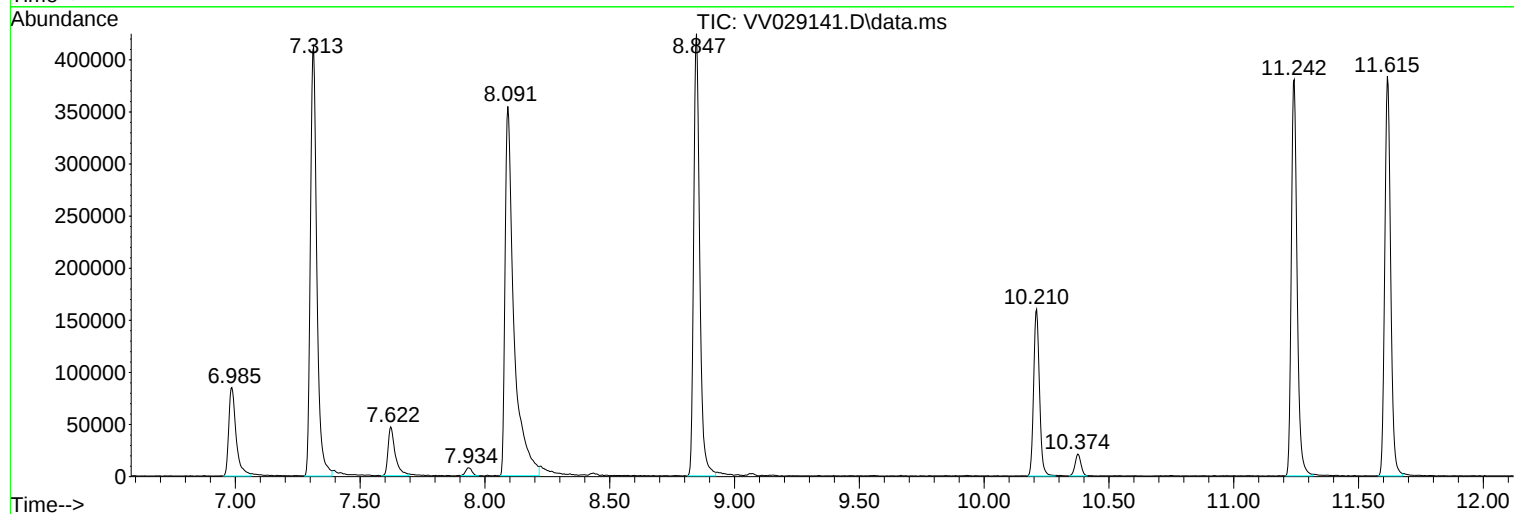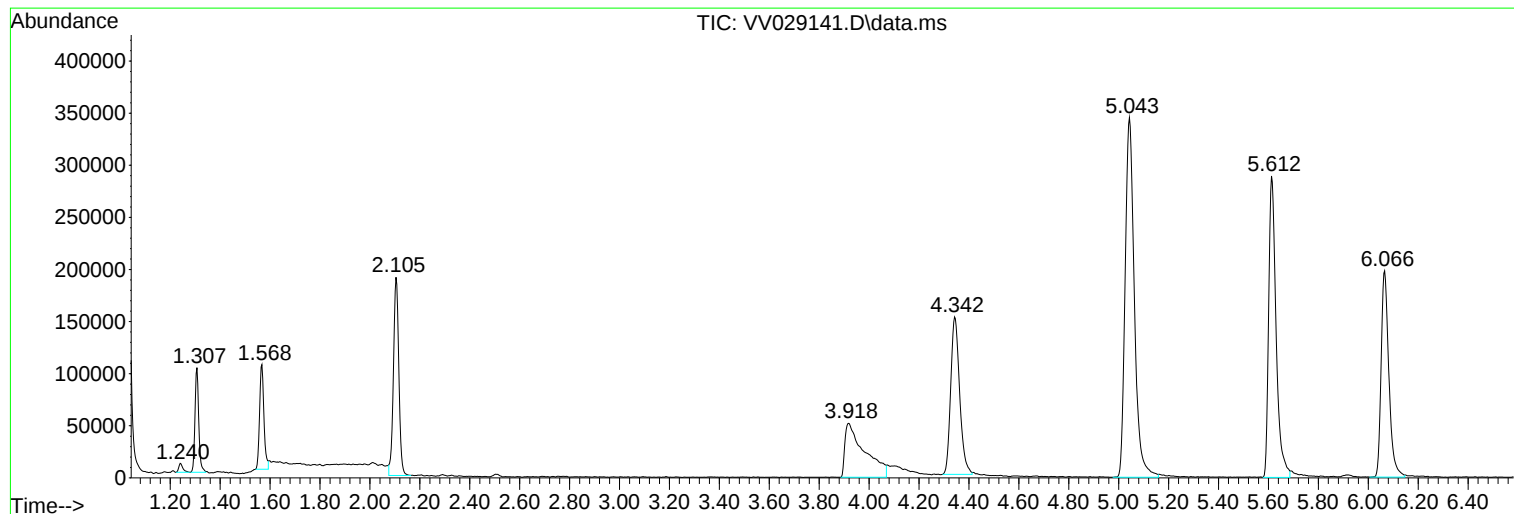

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029141.D
Acq On : 19 Nov 2022 01:13
Operator : SY/MD
Sample : N5688-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029141.D
Acq On : 19 Nov 2022 01:13
Operator : SY/MD
Sample : N5688-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc