

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029142.D
 Acq On : 19 Nov 2022 01:37
 Operator : SY/MD
 Sample : N5688-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCG7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	21	25	36	rVB	9944	10425	1.16%	0.143%
2	1.240	56	62	74	rVV	15936	18162	2.03%	0.249%
3	1.307	75	83	101	rVB	98488	111779	12.48%	1.530%
4	1.568	156	164	174	rBV	97519	111326	12.43%	1.524%
5	2.108	322	332	354	rVB	193902	292886	32.71%	4.010%
6	3.908	881	892	934	rBV2	45697	213670	23.86%	2.925%
7	4.343	1013	1027	1056	rVB2	148494	392361	43.82%	5.372%
8	5.043	1229	1245	1276	rBV2	341215	864003	96.50%	11.829%
9	5.613	1410	1422	1458	rBV	291584	617669	68.98%	8.457%
10	5.918	1505	1517	1533	rBV4	19223	41690	4.66%	0.571%
11	6.066	1549	1563	1593	rBV	198078	417708	46.65%	5.719%
12	6.985	1835	1849	1877	rBV	85469	171811	19.19%	2.352%
13	7.310	1936	1950	1976	rBV	401145	729781	81.50%	9.992%
14	7.622	2036	2047	2070	rBV	46030	90965	10.16%	1.245%
15	8.092	2182	2193	2253	rBV3	277410	895384	100.00%	12.259%
16	8.847	2417	2428	2459	rBV	426999	731363	81.68%	10.013%
17	10.210	2840	2852	2873	rBV	149275	253743	28.34%	3.474%
18	10.378	2893	2904	2916	rVB2	12695	20440	2.28%	0.280%
19	11.243	3161	3173	3200	rBV	415752	668370	74.65%	9.151%
20	11.616	3277	3289	3312	rBV	396418	650313	72.63%	8.904%




Sum of corrected areas: 7303849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029142.D
Acq On : 19 Nov 2022 01:37
Operator : SY/MD
Sample : N5688-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

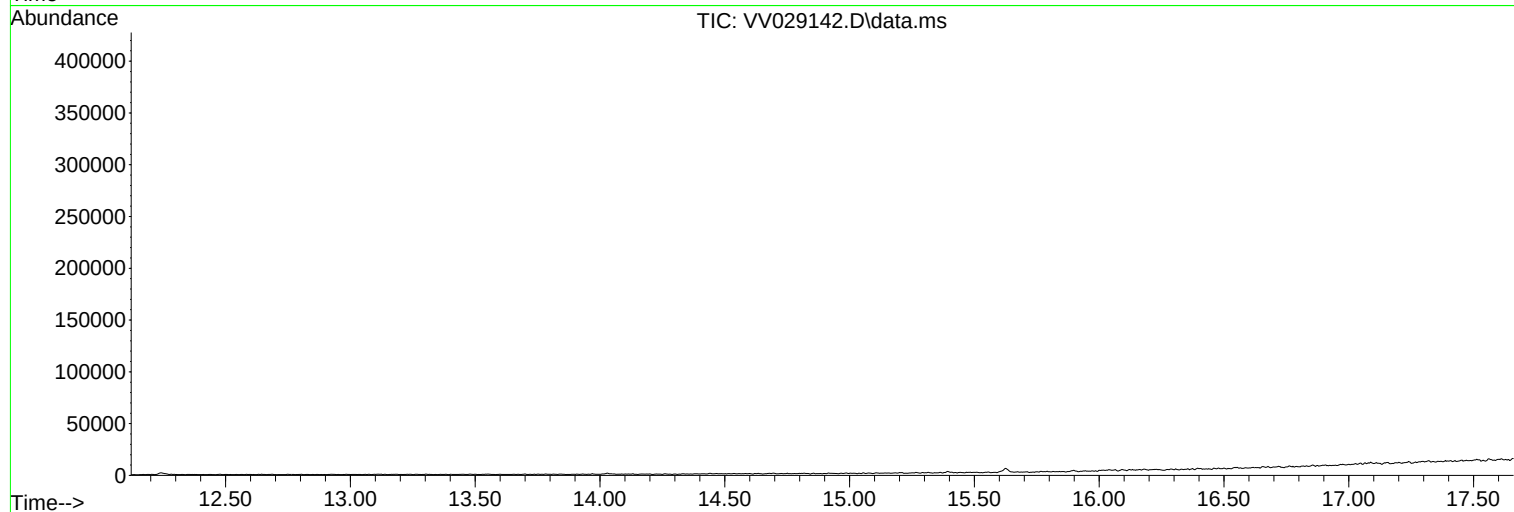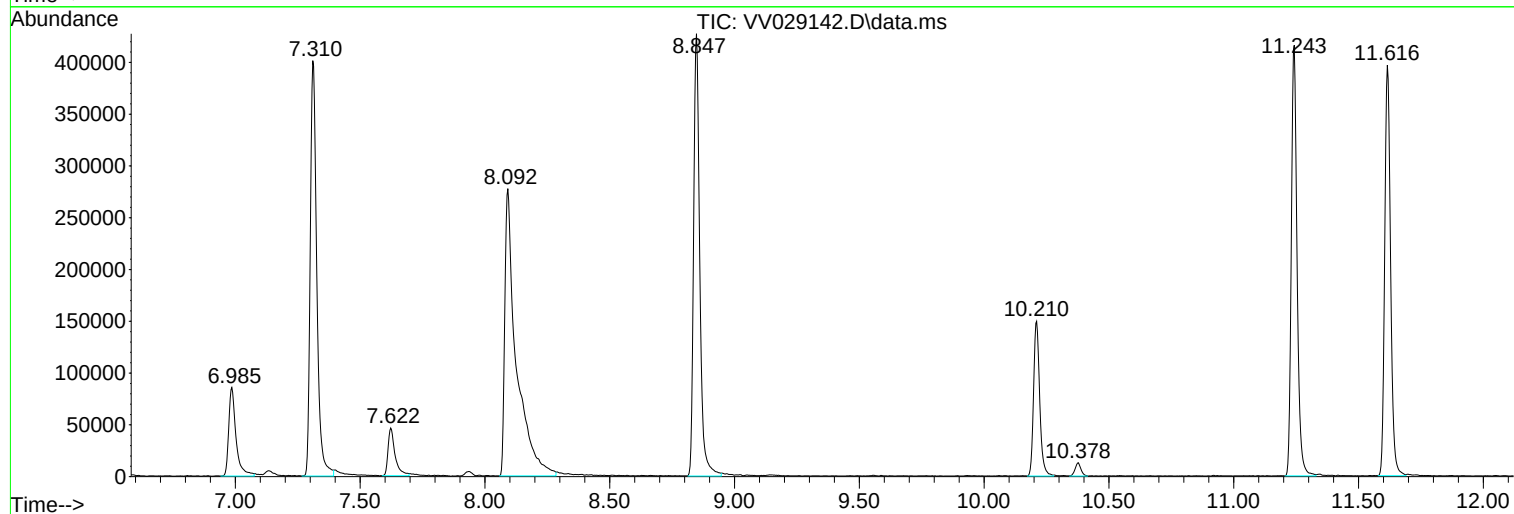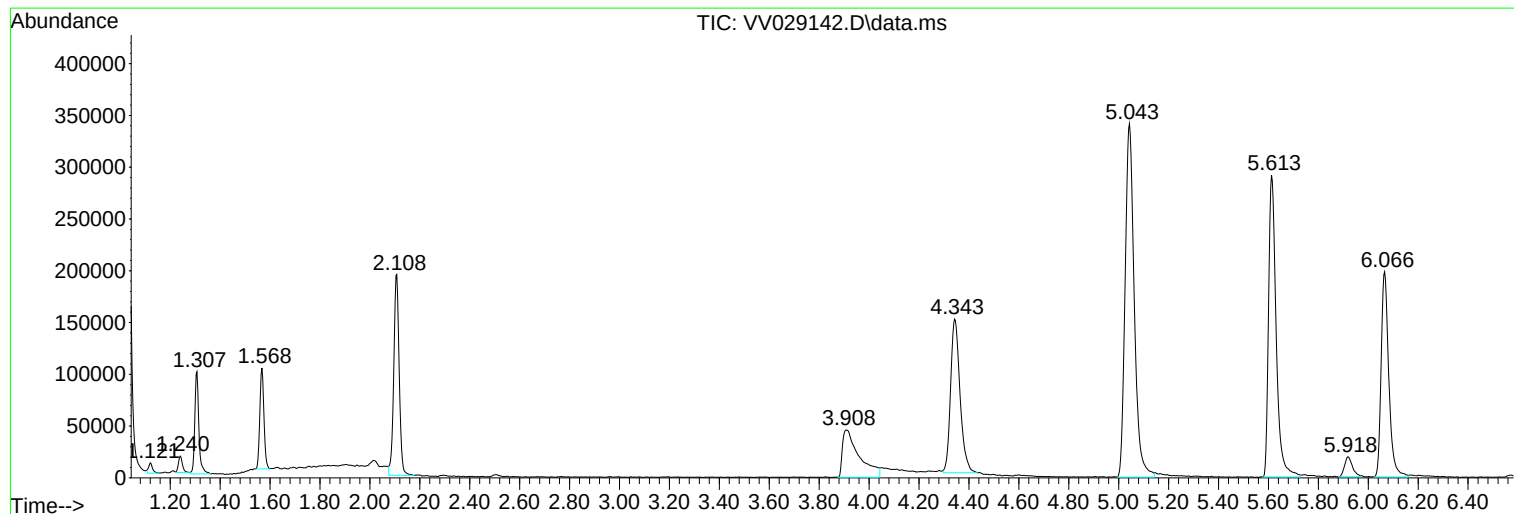

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029142.D
Acq On : 19 Nov 2022 01:37
Operator : SY/MD
Sample : N5688-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029142.D
Acq On : 19 Nov 2022 01:37
Operator : SY/MD
Sample : N5688-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc