

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029150.D
 Acq On : 19 Nov 2022 04:53
 Operator : SY/MD
 Sample : N5666-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rBV	98696	103541	11.00%	1.203%
2	1.568	146	164	177	rBV2	106217	171594	18.23%	1.994%
3	2.108	322	332	347	rVB3	210347	339383	36.06%	3.944%
4	2.503	446	455	467	rBV2	11183	19283	2.05%	0.224%
5	3.185	647	667	692	rBV	317569	675410	71.77%	7.850%
6	3.908	879	892	924	rBV4	128249	441889	46.95%	5.136%
7	4.342	1011	1027	1053	rBV	151022	391558	41.61%	4.551%
8	4.603	1089	1108	1129	rBV2	72566	187745	19.95%	2.182%
9	5.043	1228	1245	1270	rBV2	342922	873873	92.86%	10.156%
10	5.612	1410	1422	1454	rBV	302903	640750	68.09%	7.447%
11	6.066	1549	1563	1592	rBV	201029	425740	45.24%	4.948%
12	6.985	1838	1849	1881	rBV2	85306	170580	18.13%	1.983%
13	7.310	1939	1950	1972	rBV	397889	718761	76.37%	8.354%
14	7.622	2036	2047	2073	rBV	47983	93057	9.89%	1.082%
15	7.937	2133	2145	2157	rBV3	10264	19482	2.07%	0.226%
16	8.088	2179	2192	2231	rBV2	355940	941095	100.00%	10.938%
17	8.847	2416	2428	2466	rBV	452829	754771	80.20%	8.772%
18	10.210	2839	2852	2873	rBV	165290	269231	28.61%	3.129%
19	10.378	2892	2904	2918	rVB	32323	53490	5.68%	0.622%
20	11.242	3162	3173	3196	rBV	419723	675336	71.76%	7.849%
21	11.615	3277	3289	3315	rBV	393174	637600	67.75%	7.410%




Sum of corrected areas: 8604169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029150.D
Acq On : 19 Nov 2022 04:53
Operator : SY/MD
Sample : N5666-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

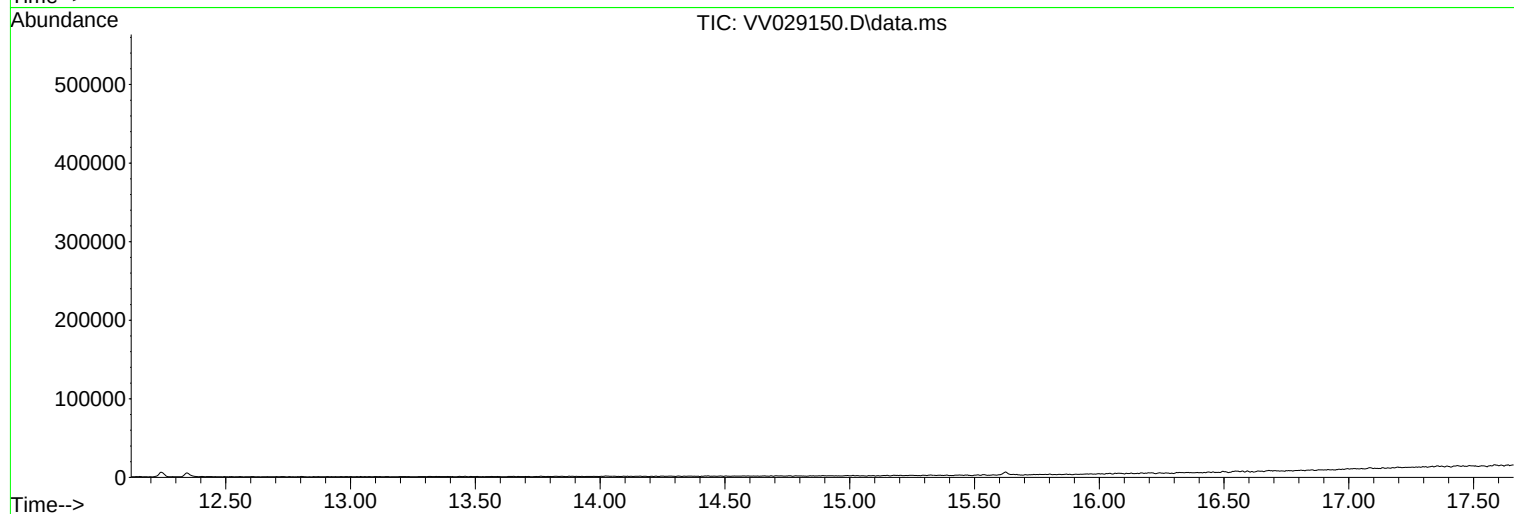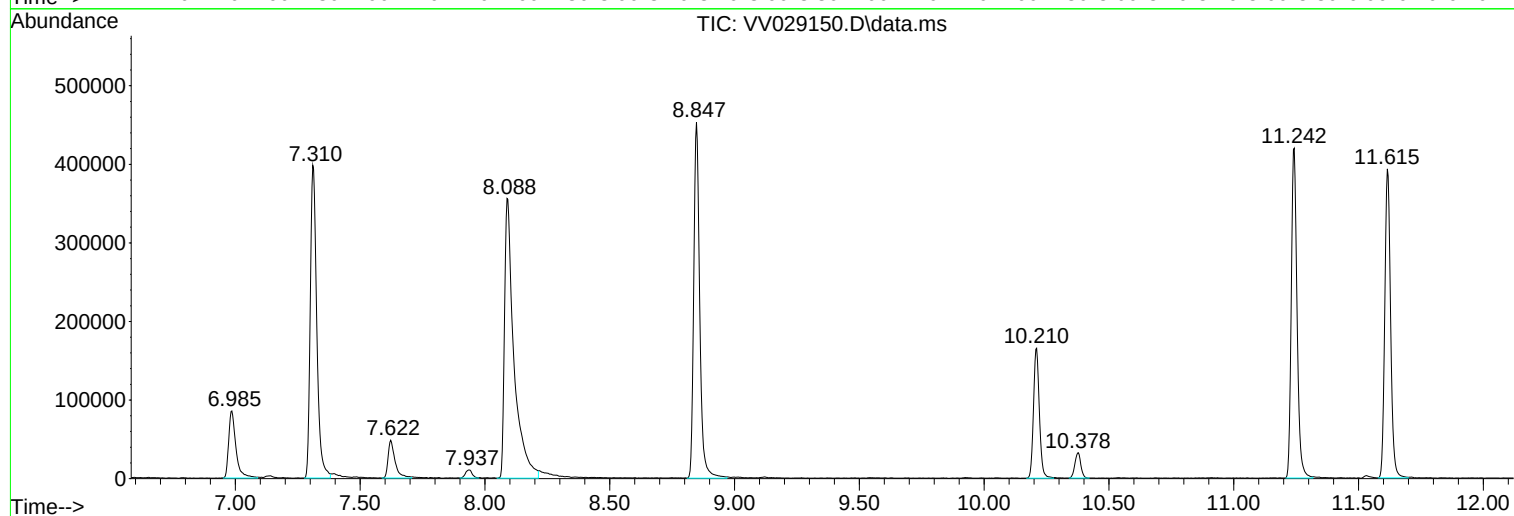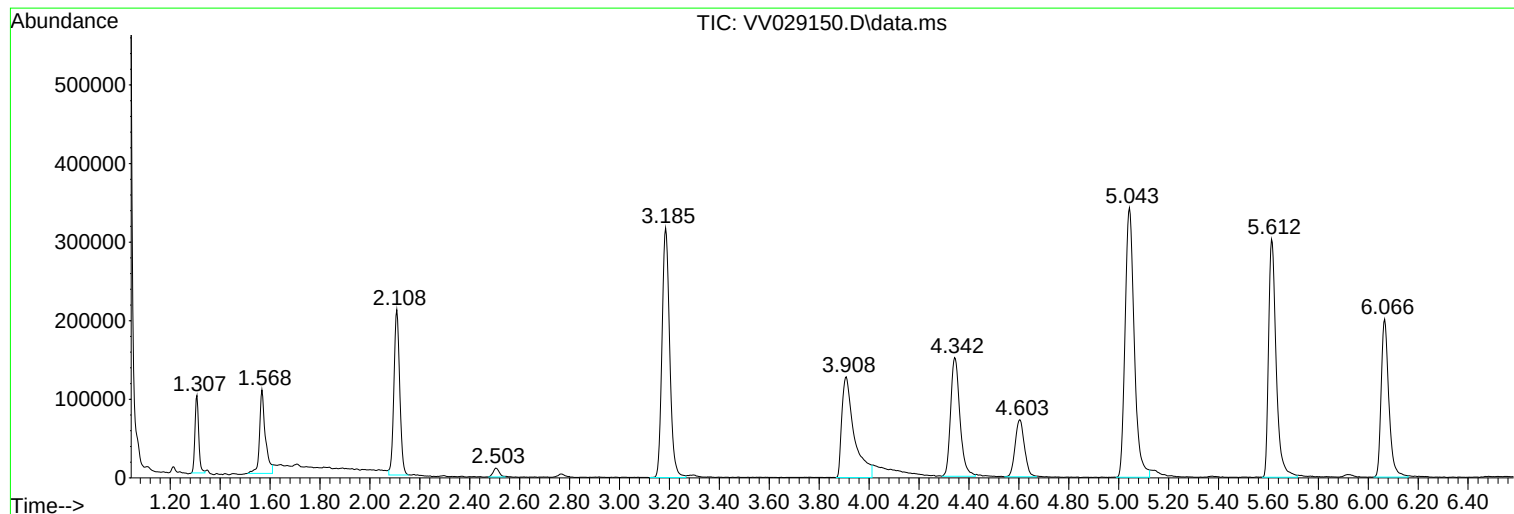

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029150.D
Acq On : 19 Nov 2022 04:53
Operator : SY/MD
Sample : N5666-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029150.D
Acq On : 19 Nov 2022 04:53
Operator : SY/MD
Sample : N5666-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc