

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029154.D
 Acq On : 19 Nov 2022 06:31
 Operator : SY/MD
 Sample : N5666-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	103	rBV	173091	187476	17.73%	2.187%
2	1.500	124	143	144	rBV2	11426	20573	1.95%	0.240%
3	1.568	157	164	177	rVB	143386	165040	15.61%	1.925%
4	2.105	320	331	347	rVB	297170	443077	41.91%	5.168%
5	3.899	876	889	923	rBV	68742	280833	26.56%	3.276%
6	4.343	1011	1027	1052	rBV	171759	438241	41.45%	5.112%
7	5.043	1229	1245	1279	rBV2	418666	1057257	100.00%	12.332%
8	5.613	1406	1422	1457	rBV	356563	748153	70.76%	8.727%
9	6.066	1549	1563	1592	rBV	229090	484092	45.79%	5.647%
10	6.982	1834	1848	1878	rBV	96221	194069	18.36%	2.264%
11	7.310	1937	1950	1992	rBV	512697	935752	88.51%	10.915%
12	7.622	2037	2047	2075	rBV2	51442	103779	9.82%	1.210%
13	7.934	2134	2144	2155	rBV	9663	16815	1.59%	0.196%
14	8.088	2181	2192	2239	rBV2	340071	851062	80.50%	9.927%
15	8.847	2415	2428	2452	rBV	520880	879332	83.17%	10.257%
16	10.207	2835	2851	2873	rBV	154184	253756	24.00%	2.960%
17	10.378	2893	2904	2918	rVB2	31110	52214	4.94%	0.609%
18	11.239	3160	3172	3196	rBV	479827	771462	72.97%	8.998%
19	11.616	3277	3289	3314	rBV	422611	690317	65.29%	8.052%




Sum of corrected areas: 8573300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029154.D
Acq On : 19 Nov 2022 06:31
Operator : SY/MD
Sample : N5666-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

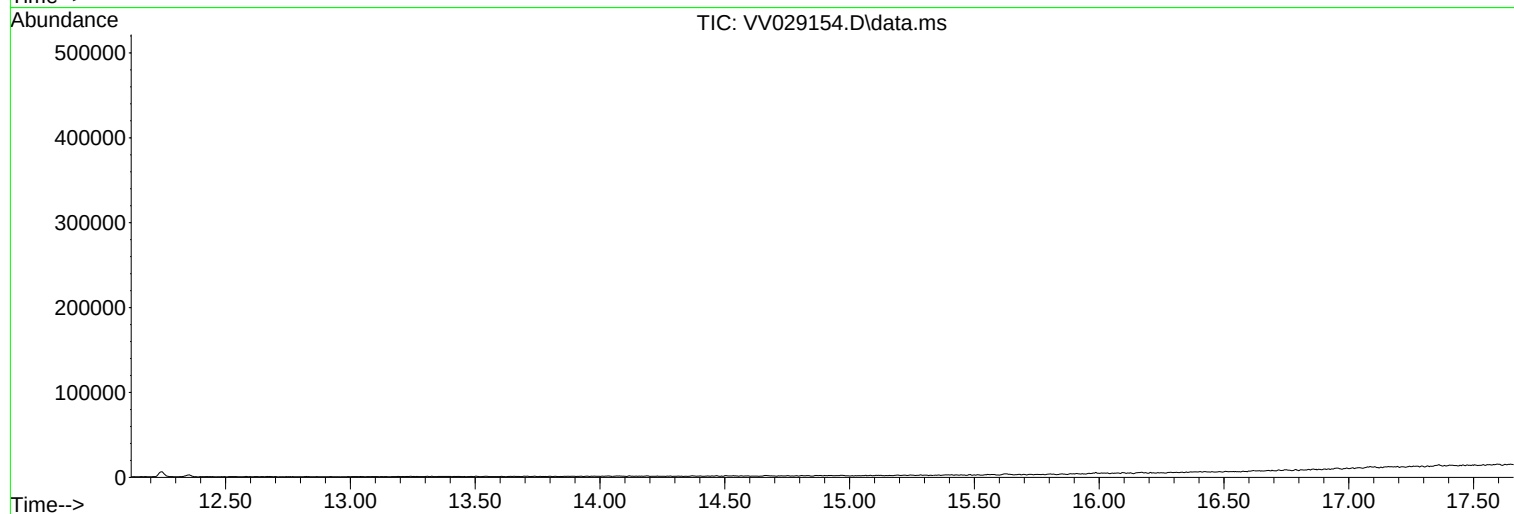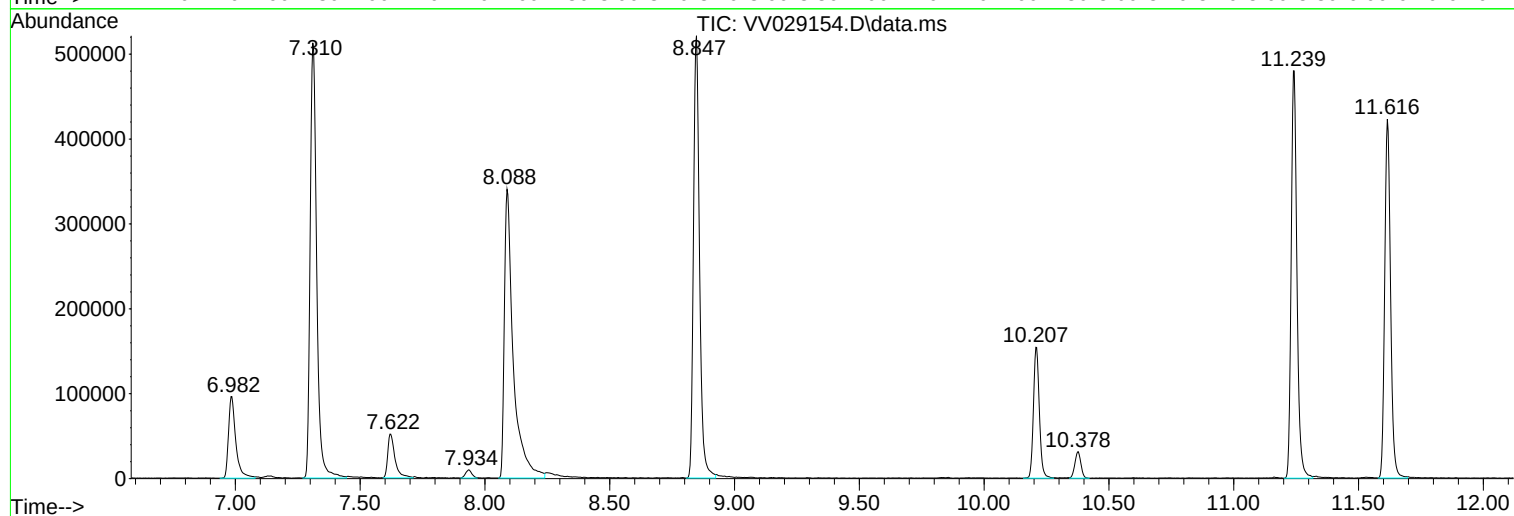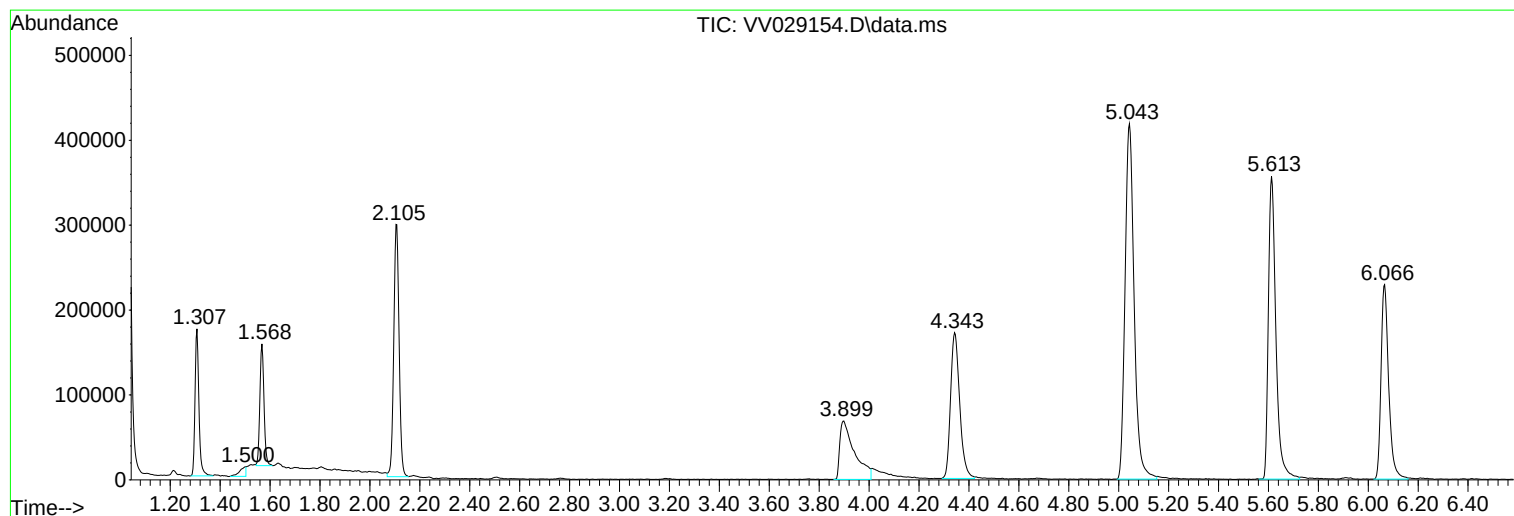

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029154.D
Acq On : 19 Nov 2022 06:31
Operator : SY/MD
Sample : N5666-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029154.D
Acq On : 19 Nov 2022 06:31
Operator : SY/MD
Sample : N5666-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc