
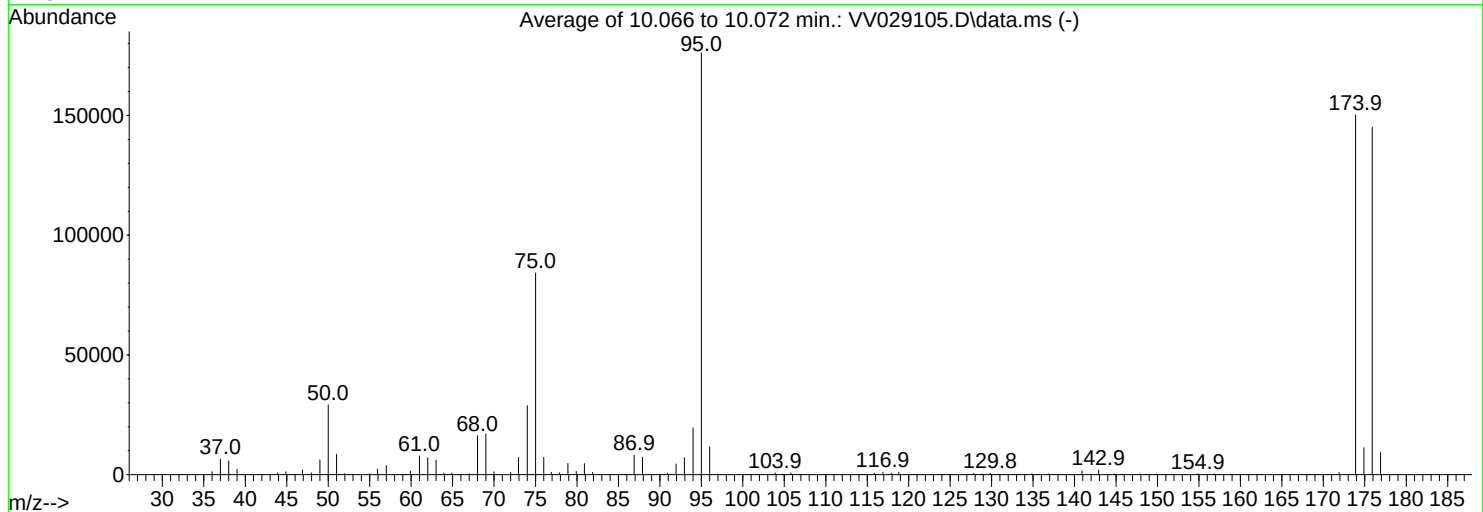


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029105.D
 Acq On : 18 Nov 2022 09:49
 Operator : SY/MD
 Sample : BFB399
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB399

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 18 04:35:43 2022

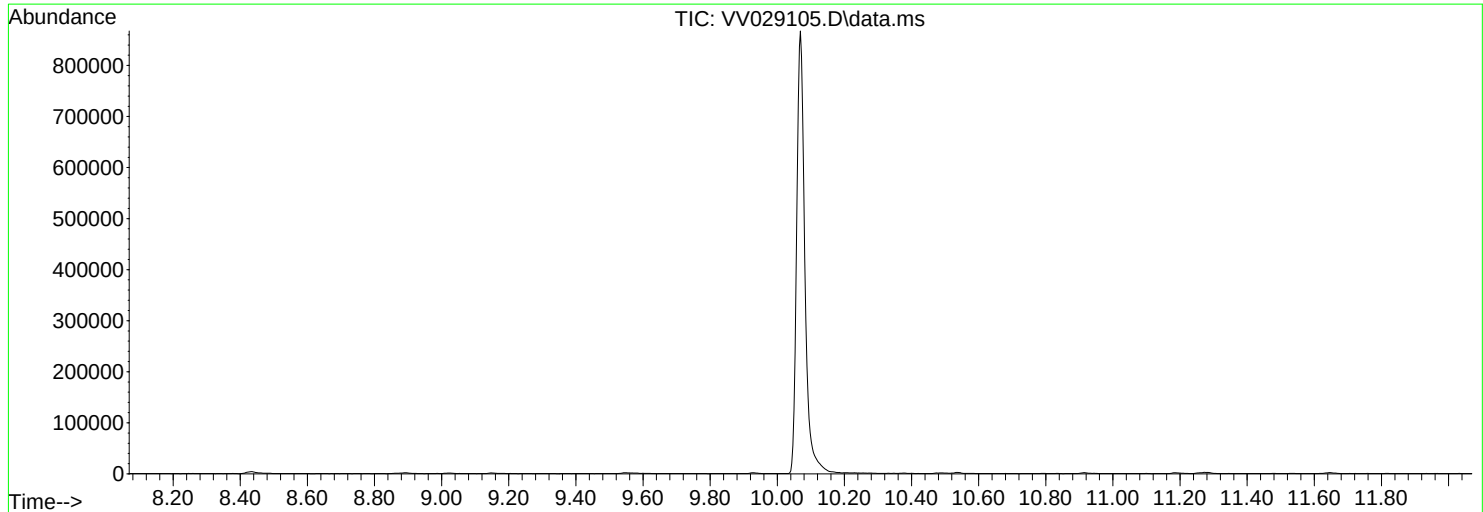

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	29195	PASS
75	95	30	80	47.8	84216	PASS
95	95	100	100	100.0	176149	PASS
96	95	5	9	6.6	11620	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.3	150208	PASS
175	174	5	9	7.5	11235	PASS
176	174	95	105	96.6	145109	PASS
177	176	5	10	6.3	9212	PASS

m/z	Abundance
40.00	243.0
43.90	374.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
36.00	1261.0
37.00	6708.0
38.00	5540.0
39.00	2341.0
39.90	383.0
43.90	1176.0
44.90	1239.0
45.90	137.0
46.90	2069.0
48.00	761.0
49.00	6270.0
50.00	29968.0
51.00	8640.0
51.90	388.0
53.00	109.0
55.00	452.0
56.00	2343.0
57.00	3802.0
57.90	187.0
59.90	1523.0
61.00	7924.0
62.00	7543.0
63.00	6216.0
63.90	737.0
64.90	766.0
65.80	121.0
67.00	352.0
68.00	16271.0
69.00	16992.0
70.00	1209.0
72.00	1027.0
73.00	7231.0
74.00	28944.0
75.00	84408.0
76.00	7443.0
76.90	1009.0
77.90	667.0
78.90	4991.0
79.90	1373.0
80.90	4624.0
81.90	922.0
82.80	168.0
85.80	222.0
86.90	8182.0
87.90	7214.0
90.90	654.0
92.00	4572.0
92.90	7018.0
94.00	20000.0
95.00	175808.0
96.00	11922.0
97.00	347.0
103.90	752.0
104.80	283.0
105.80	820.0
106.80	169.0
109.80	119.0
110.80	144.0
111.90	102.0
112.80	119.0
114.90	159.0
115.80	626.0
116.90	1080.0
117.90	590.0
118.80	957.0
124.80	105.0
127.80	533.0
128.80	302.0
129.80	533.0
130.80	262.0
134.80	378.0
136.90	303.0
139.80	147.0
140.90	1579.0
142.00	219.0
142.90	1846.0
144.80	319.0
145.70	215.0
147.90	343.0
149.80	179.0
151.90	147.0
153.00	164.0
154.90	464.0
156.90	324.0
158.80	236.0
161.00	148.0
170.90	123.0
171.90	824.0
173.90	147200.0
174.90	11215.0
175.90	141056.0
176.90	9309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

177.90

240.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
36.00	1242.0
37.00	6657.0
38.00	5888.0
39.00	2227.0
39.90	331.0
43.90	1176.0
44.90	1214.0
45.90	164.0
46.90	2040.0
48.00	761.0
49.00	6456.0
50.00	30176.0
51.00	8789.0
51.90	418.0
52.90	150.0
55.00	475.0
55.90	2395.0
57.00	3935.0
57.90	221.0
59.90	1493.0
61.00	7993.0
62.00	7249.0
63.00	6287.0
64.00	676.0
64.90	661.0
65.80	113.0
67.10	394.0
68.00	16904.0
69.00	17552.0
70.00	1258.0
72.00	958.0
72.90	7403.0
74.00	29784.0
75.00	86864.0
76.00	7423.0
76.90	1047.0
77.90	756.0
78.90	4823.0
79.90	1418.0
80.90	4677.0
81.90	982.0
82.80	181.0
85.90	212.0
86.90	8514.0
87.90	7501.0
90.90	671.0
92.00	4639.0
93.00	7262.0
94.00	20064.0
95.00	181824.0
96.00	12006.0
96.90	363.0
103.90	809.0
104.80	296.0
105.80	788.0
107.00	181.0
110.90	151.0
111.90	121.0
112.90	145.0
114.70	123.0
115.80	627.0
116.90	1146.0
117.90	606.0
118.80	946.0
124.80	108.0
127.80	579.0
128.80	360.0
129.80	576.0
130.80	257.0
134.80	428.0
136.90	348.0
139.90	148.0
140.90	1639.0
142.10	253.0
142.90	1966.0
144.80	315.0
145.80	211.0
147.00	124.0
147.90	377.0
149.80	219.0
151.90	130.0
153.00	172.0
154.90	437.0
156.00	104.0
156.80	330.0
158.80	280.0
161.00	128.0
170.90	140.0
171.90	888.0
173.90	155264.0
174.90	11577.0
175.90	149760.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

176.909371.0

177.90232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
36.00	1067.0
37.00	6108.0
38.00	5768.0
39.00	2029.0
39.80	307.0
43.90	1046.0
44.90	1079.0
45.90	149.0
46.90	1738.0
47.90	700.0
49.00	5908.0
50.00	27440.0
51.00	8207.0
52.00	406.0
52.90	153.0
55.00	448.0
55.90	2305.0
57.00	3785.0
57.90	208.0
59.90	1323.0
61.00	7627.0
62.00	6463.0
63.00	5685.0
64.00	617.0
64.90	522.0
67.10	390.0
68.00	15649.0
69.00	16488.0
70.00	1231.0
72.00	856.0
73.00	7075.0
74.00	27696.0
75.00	81376.0
76.00	6751.0
76.90	998.0
77.90	747.0
78.90	4244.0
79.90	1310.0
80.90	4483.0
81.90	884.0
82.80	156.0
85.80	210.0
86.90	7825.0
87.90	7092.0
90.90	607.0
91.90	4230.0
93.00	6768.0
94.00	18512.0
95.00	170816.0
96.00	10933.0
96.90	319.0
103.90	752.0
104.80	265.0
105.80	660.0
107.00	146.0
110.90	156.0
111.90	125.0
112.90	144.0
114.80	116.0
115.90	561.0
116.90	1088.0
117.90	592.0
118.80	866.0
127.90	549.0
128.90	385.0
129.90	610.0
130.80	220.0
134.90	399.0
136.90	338.0
139.90	120.0
140.90	1557.0
142.00	257.0
142.90	1841.0
144.80	298.0
145.80	206.0
147.00	143.0
147.90	375.0
149.90	225.0
152.90	154.0
154.90	405.0
156.00	129.0
156.80	301.0
158.80	268.0
160.70	132.0
170.90	133.0
171.90	857.0
173.90	148160.0
174.90	10912.0
175.90	144512.0
176.90	8956.0
177.90	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399