


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111825\
Data File : VV039396.D
Acq On : 18 Nov 2025 09:31
Operator : SY/MD
Sample : BFB208
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB208

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Nov 19 01:11:25 2025

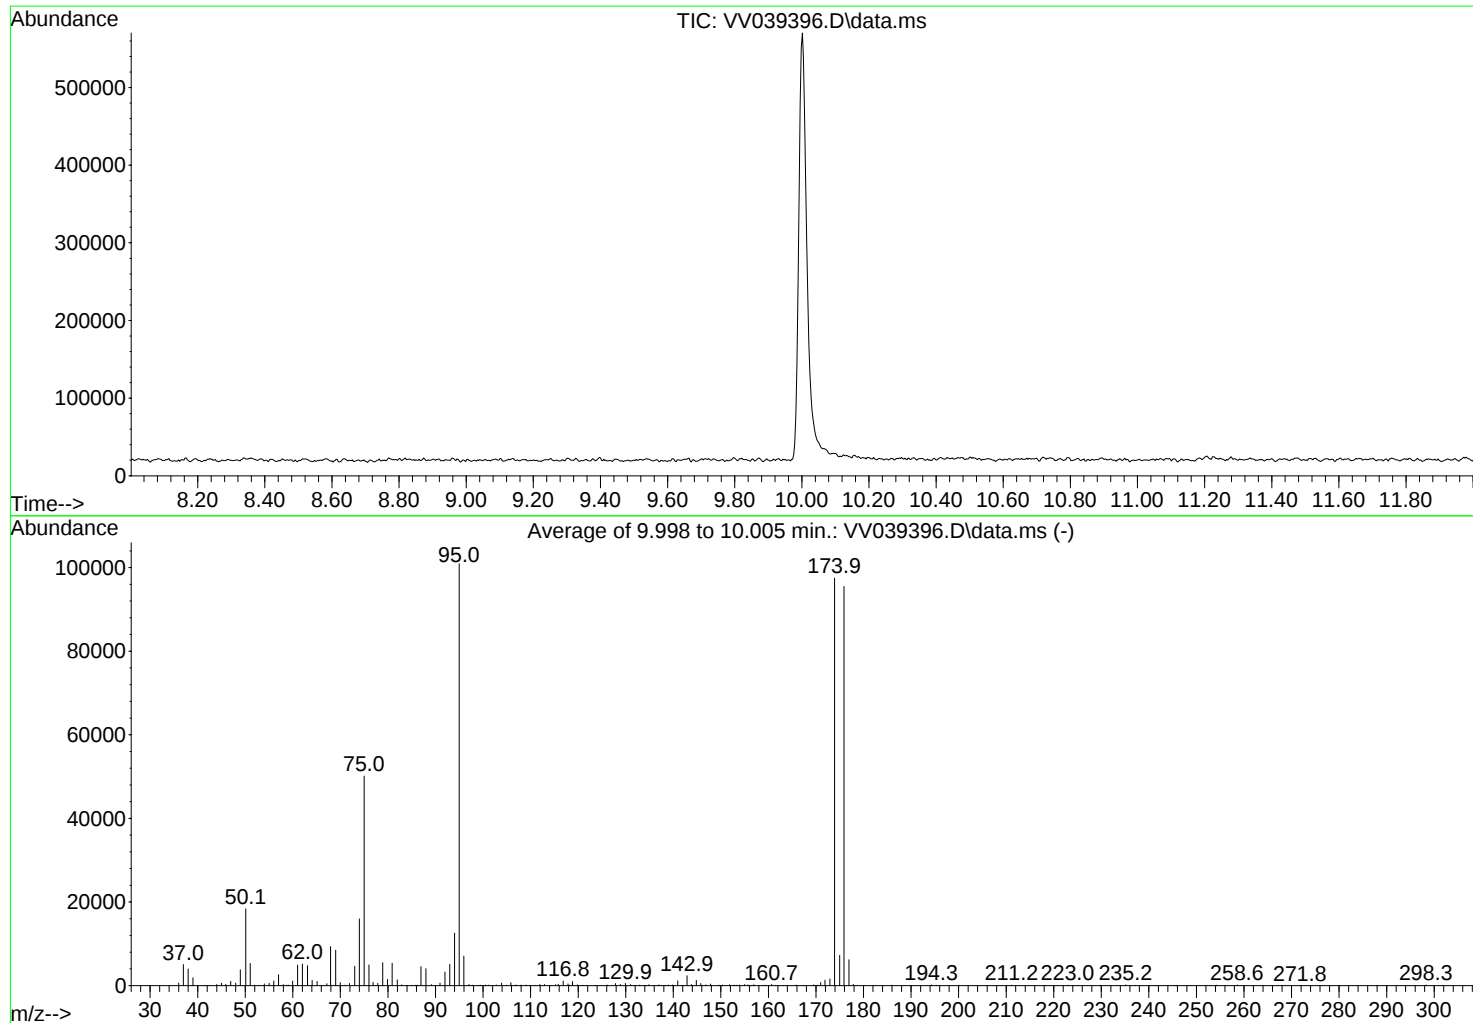

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2772

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	18.2	18355	PASS
75	95	30	66	49.7	50115	PASS
95	95	100	100	100.0	100916	PASS
96	95	5	9	7.0	7080	PASS
173	174	0.00	2	1.6	1589	PASS
174	95	50	120	96.6	97502	PASS
175	174	4	9	7.4	7208	PASS
176	174	93	101	98.0	95504	PASS
177	176	5	9	6.5	6169	PASS

Average of 9.998 to 10.005 min.: VV039396.D\data.ms

BFB208

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	614	48.00	593	58.75	89	69.00	8453
37.00	5021	48.95	3774	59.05	91	70.00	700
38.00	3976	50.10	18355	59.95	1101	71.00	90
39.00	1865	51.05	5301	61.00	4881	71.90	462
41.50	65	52.00	118	62.00	5132	73.00	4603
42.05	75	52.90	77	63.10	4766	74.00	15946
42.50	61	54.00	392	64.05	1257	75.00	50115
44.00	242	55.00	551	65.10	963	76.00	4966
45.00	559	56.00	1082	66.00	59	76.90	761
45.90	248	57.00	2592	67.15	459	77.85	512
46.95	1028	58.00	245	67.95	9331	78.90	5470

Average of 9.998 to 10.005 min.: VV039396.D\data.ms

BFB208

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	1487	90.95	612	101.20	104	109.70	59
80.90	5341	92.00	3236	101.50	38	110.90	65
81.95	1358	93.00	5095	102.80	151	111.95	267
82.90	177	94.00	12532	103.90	585	112.90	239
84.00	51	95.00	100916	104.95	92	114.30	34
85.00	45	95.95	7080	105.85	683	115.25	210
85.85	100	97.05	270	106.90	120	115.80	338
86.20	81	97.80	117	107.10	65	116.85	1087
86.95	4523	99.00	39	107.90	61	117.85	406
88.00	4029	99.40	112	108.10	96	118.20	103
89.15	222	100.55	132	109.05	145	118.80	995

Average of 9.998 to 10.005 min.: VV039396.D\data.ms

BFB208

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.85	182	134.90	223	143.80	232	153.40	81
121.00	79	136.70	76	144.85	1241	153.90	148
123.45	15	137.00	159	145.80	474	155.00	264
126.10	138	137.55	35	146.85	186	155.70	160
127.85	466	138.30	79	147.85	360	156.50	60
128.85	286	138.95	136	149.60	109	156.95	222
129.95	519	139.85	123	149.80	35	157.90	39
131.00	203	140.95	1144	150.35	120	158.80	41
131.95	68	141.70	64	151.85	197	159.30	87
132.90	117	142.05	74	152.60	77	160.70	284
134.30	35	142.90	2360	152.85	115	161.55	72

Average of 9.998 to 10.005 min.: VV039396.D\data.ms

BFB208

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
161.90	36	175.00	7208	218.20	37	248.80	36
163.20	35	175.90	95504	223.00	95	254.20	80
164.05	77	176.95	6169	225.10	36	258.60	140
165.85	132	177.85	280	229.90	101	267.90	74
167.30	41	185.90	85	233.30	43	271.80	40
169.55	162	194.30	164	235.15	168	287.90	77
170.35	111	195.40	41	237.20	76	295.80	37
171.00	727	200.10	92	241.50	39	298.30	136
171.90	1294	207.40	35	243.40	35		
172.95	1589	210.30	35	245.50	35		
173.90	97502	211.20	83	245.85	79		

Instrument :

MSVOA_V

ClientSampleId :

BFB208