


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111918\
 Data File : VV008639.D
 Acq On : 19 Nov 2018 09:16
 Operator : SY/MD
 Sample : BFB50
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB50

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 20 06:56:52 2018

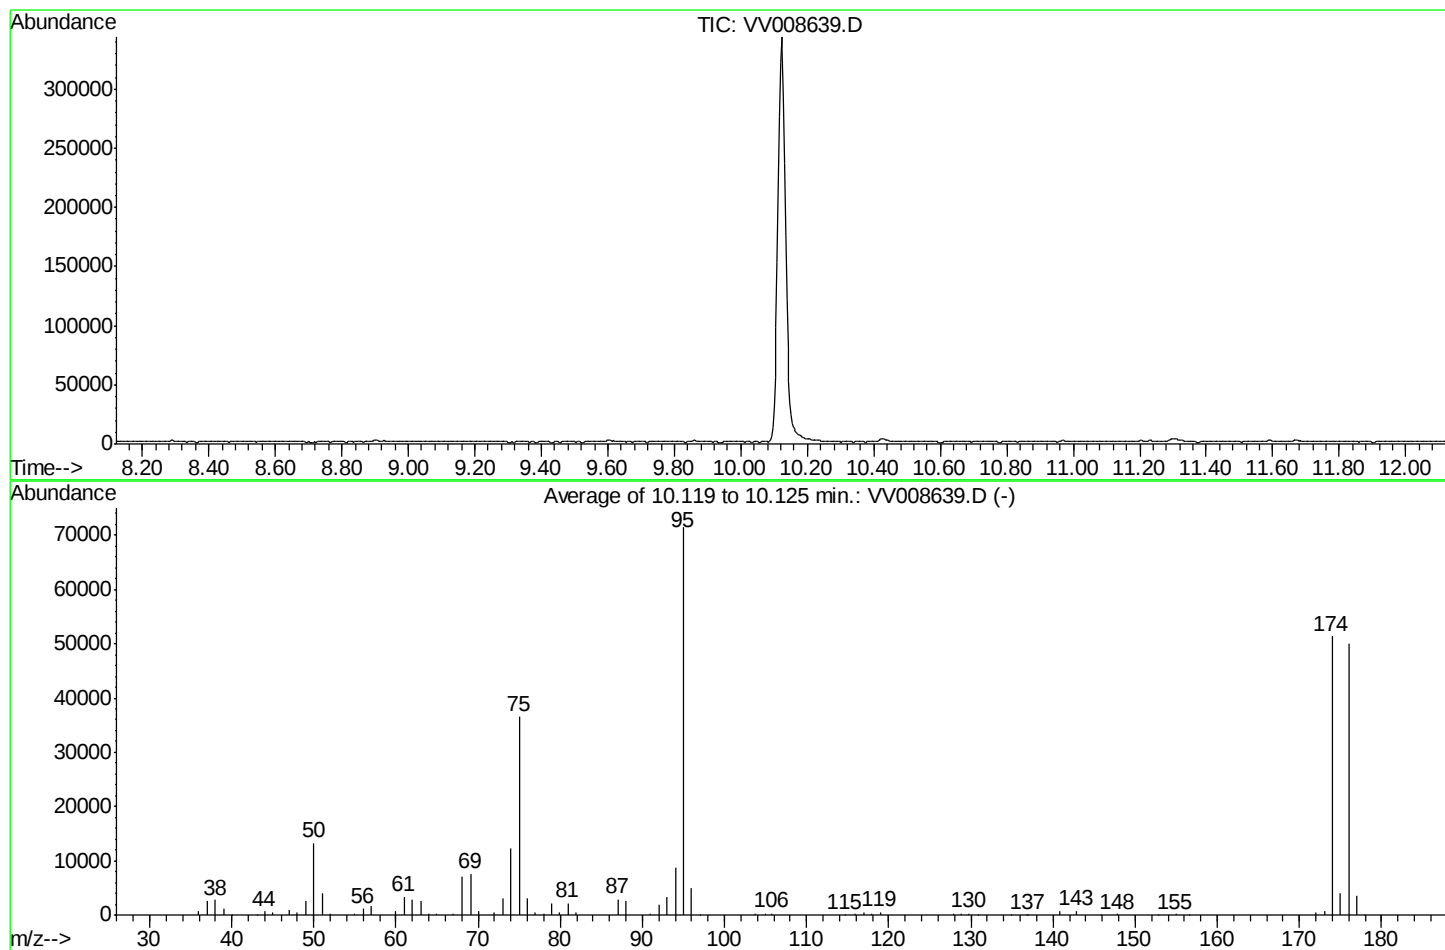

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	13232	PASS
75	95	30	80	51.1	36504	PASS
95	95	100	100	100.0	71480	PASS
96	95	5	9	7.0	4976	PASS
173	174	0.00	2	1.2	616	PASS
174	95	50	120	71.9	51384	PASS
175	174	5	9	7.9	4051	PASS
176	174	95	101	97.4	50045	PASS
177	176	5	9	7.0	3507	PASS

m/z	Abundance
39.90	376.0
44.00	1368.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
35.90	648.0
37.00	2681.0
38.00	2700.0
39.00	1127.0
39.90	504.0
43.10	124.0
44.00	1740.0
44.90	568.0
47.00	948.0
48.00	388.0
49.00	2596.0
50.00	13057.0
51.00	4005.0
51.90	219.0
55.00	180.0
56.00	1149.0
57.00	1707.0
60.00	725.0
61.00	3193.0
62.00	2953.0
63.00	2387.0
64.00	284.0
64.90	312.0
67.00	205.0
68.00	6990.0
69.10	7496.0
70.00	589.0
72.00	438.0
73.00	3179.0
74.00	11740.0
75.00	36072.0
76.00	3155.0
76.90	517.0
78.00	258.0
78.90	2072.0
79.90	455.0
80.90	2023.0
82.00	408.0
87.00	2809.0
87.90	2671.0
90.90	261.0
92.00	1988.0
93.00	3139.0
94.00	8627.0
95.00	69584.0
96.00	4893.0
96.90	126.0
103.80	284.0
105.00	141.0
105.80	304.0
114.70	106.0
115.80	196.0
116.90	393.0
117.90	240.0
118.90	401.0
127.90	202.0
128.80	175.0
129.80	213.0
137.00	154.0
140.80	692.0
142.90	815.0
145.80	116.0
148.00	156.0
155.00	177.0
171.90	311.0
173.90	48672.0
175.00	3912.0
176.00	47728.0
177.00	3553.0
177.90	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	609.0
37.10	2756.0
38.00	2805.0
39.00	1164.0
40.00	506.0
43.20	119.0
44.00	2052.0
45.00	566.0
47.00	939.0
48.00	421.0
49.00	2673.0
50.00	13672.0
51.00	4012.0
52.00	221.0
55.00	242.0
56.00	1187.0
57.00	1810.0
60.00	777.0
61.00	3533.0
62.00	2941.0
63.00	2594.0
64.00	287.0
64.90	367.0
66.90	243.0
68.00	7411.0
69.10	7736.0
70.00	636.0
72.00	440.0
73.00	3257.0
74.00	12882.0
75.00	37680.0
76.00	3263.0
76.90	580.0
78.00	243.0
78.90	2142.0
79.90	460.0
80.90	2199.0
81.90	462.0
87.00	3056.0
88.00	2606.0
90.90	307.0
92.00	2042.0
93.00	3350.0
94.00	9042.0
95.00	73464.0
96.00	5227.0
96.90	113.0
103.80	286.0
104.90	138.0
105.80	331.0
115.80	198.0
116.90	469.0
117.90	264.0
119.00	509.0
127.90	244.0
128.80	141.0
129.80	265.0
130.90	135.0
134.80	137.0
136.90	133.0
140.80	735.0
142.90	837.0
145.80	106.0
147.80	171.0
152.80	102.0
155.00	209.0
156.60	112.0
171.90	412.0
173.10	913.0
174.00	52848.0
175.00	4182.0
176.00	51480.0
177.00	3636.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	544.0
37.00	2662.0
38.00	2697.0
39.00	1105.0
40.00	461.0
43.20	112.0
44.00	2136.0
45.00	545.0
47.00	798.0
48.00	396.0
49.00	2451.0
50.00	12968.0
51.00	3774.0
52.00	199.0
54.90	264.0
56.00	1050.0
57.00	1798.0
60.00	620.0
61.00	3494.0
62.00	2736.0
63.00	2524.0
64.00	272.0
64.90	333.0
66.90	253.0
68.00	7032.0
69.00	7459.0
70.00	606.0
72.00	393.0
73.00	3126.0
74.00	12487.0
75.00	35760.0
76.00	3053.0
76.90	574.0
78.00	218.0
78.90	1967.0
79.80	469.0
80.90	2238.0
81.90	455.0
87.00	2974.0
87.90	2264.0
90.90	313.0
92.00	1913.0
93.00	3188.0
94.00	8406.0
95.00	71392.0
96.00	4809.0
97.00	102.0
103.80	267.0
104.80	116.0
105.80	322.0
115.90	204.0
116.90	516.0
117.90	248.0
119.00	528.0
127.90	276.0
128.80	113.0
129.80	282.0
130.90	138.0
134.90	122.0
136.70	141.0
140.80	731.0
142.90	804.0
147.80	178.0
152.80	104.0
154.90	228.0
172.00	422.0
173.10	937.0
174.00	52632.0
175.00	4059.0
176.00	50928.0
177.00	3332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50