
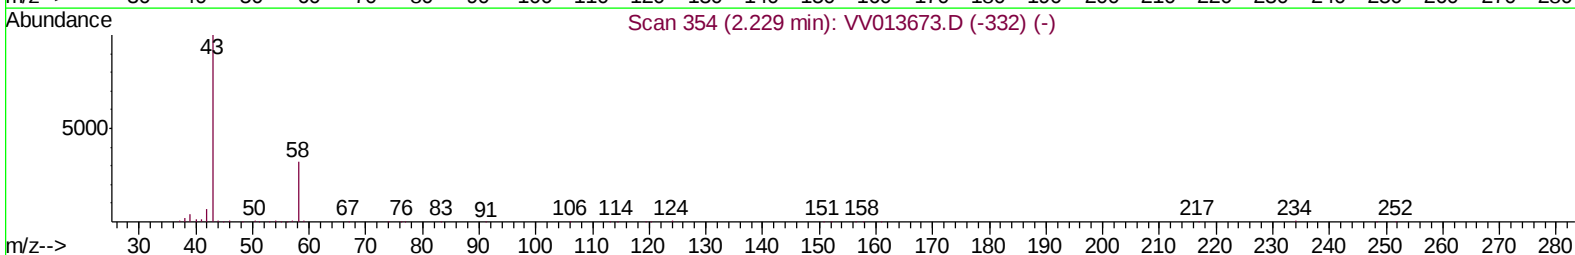
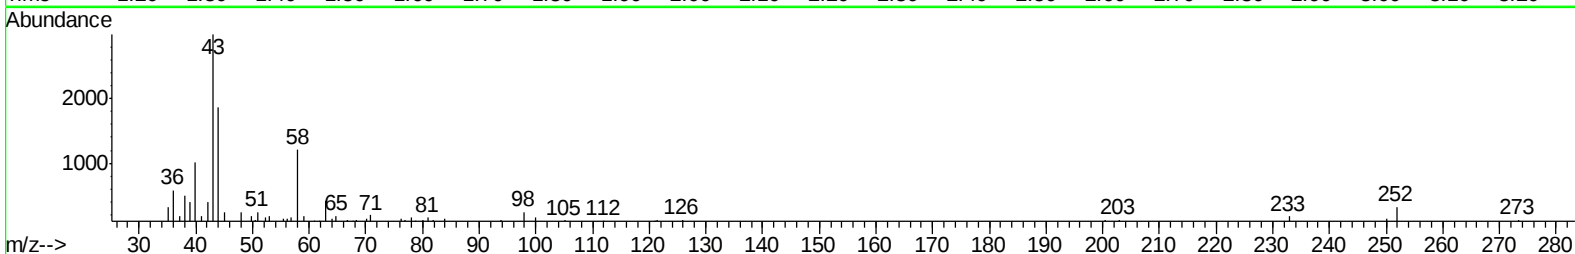


Data File : VV013677.D
Acq On : 19 Nov 2019 14:46
Operator : SY/MD
Sample : K5910-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 20 01:58:59 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 20 01:31:47 2019
Response via : Initial Calibration

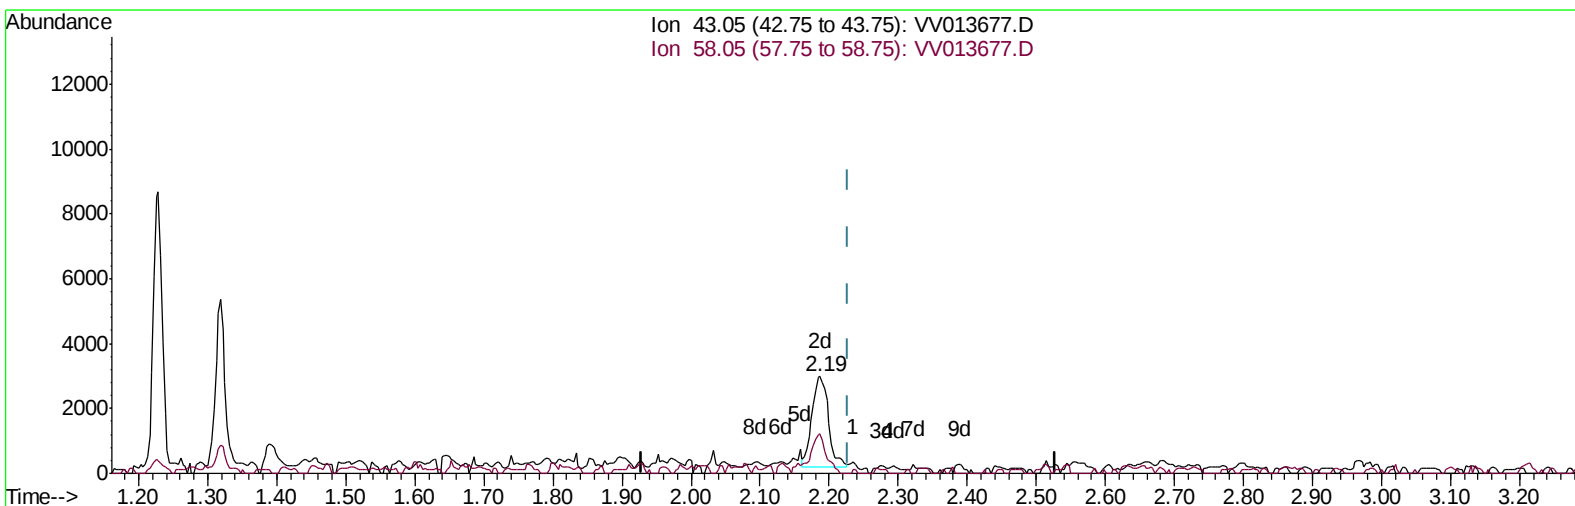

TIC: VV013677.D

(13) Acetone (T)

2.187min (-0.042) 1.47ug/L m

response 4597

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	0.00
0.00	0.00	0.00
0.00	0.00	0.00