
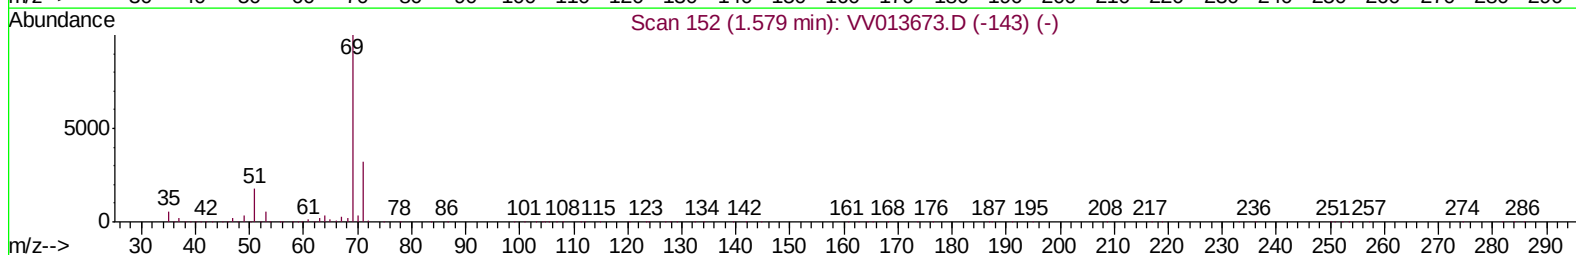
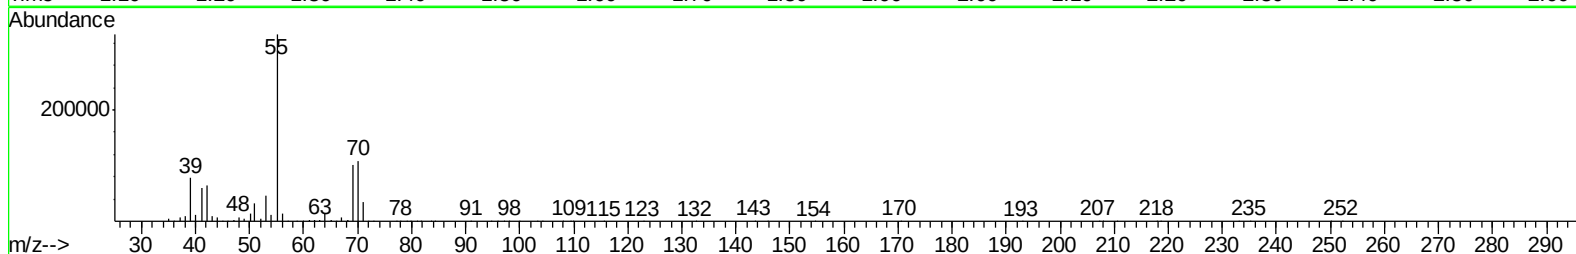


Data File : VV013679.D
Acq On : 19 Nov 2019 15:33
Operator : SY/MD
Sample : K5910-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Nov 20 01:35:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 20 01:31:47 2019
Response via : Initial Calibration

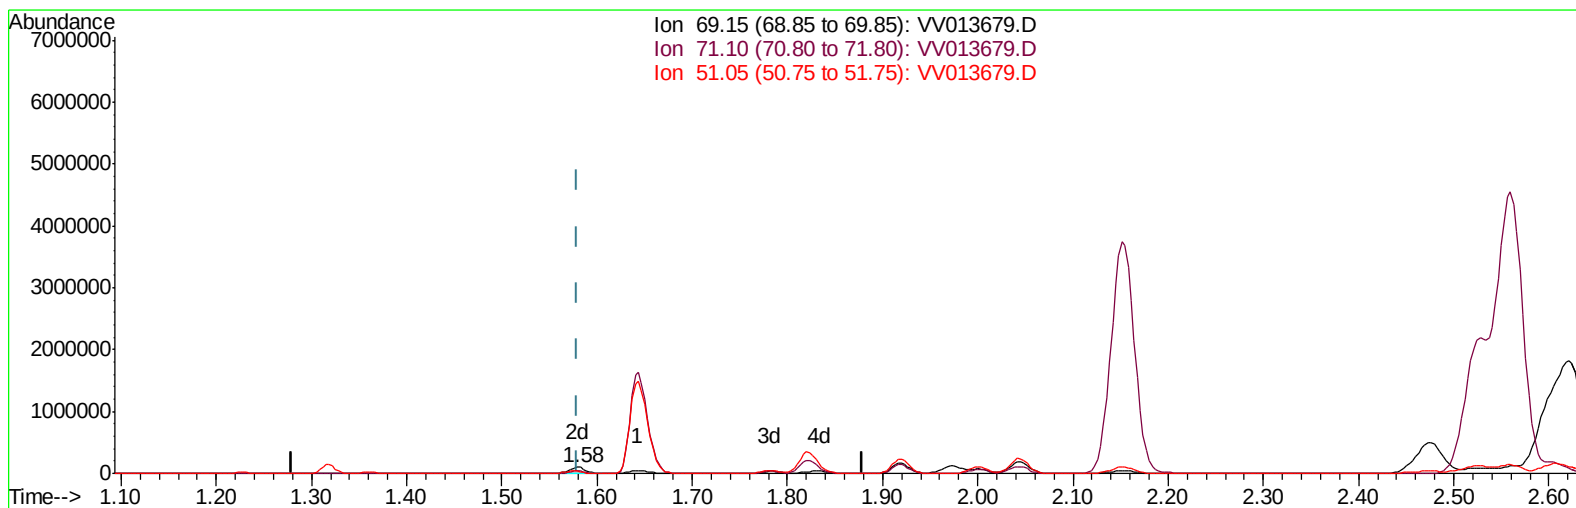

TIC: VV013679.D

(7) Chloroethane-d5 (S)

1.579min (-0.000) 4.33ug/L m

response 118545

Ion	Exp%	Act%
69.15	100	100
71.10	32.50	1767.99#
51.05	24.80	1659.02#
0.00	0.00	0.00