

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111920\
 Data File : VV019406.D
 Acq On : 19 Nov 2020 13:50
 Operator : SY/MD
 Sample : L4485-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-05

Manual Integrations
 APPROVED

MMDadoda
 11/30/2020 3:40:10 PM

Quant Time: Nov 20 11:18:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 20 00:26:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	4865	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.88	117	4473	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.28	152	2333	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.32	65	3493	0.50	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	100.00%		
4) 1,2-Dichloroethane-d4	5.07	65	2110	0.52	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	104.00%		
7) 1,2-Dichloropropane-d6	6.09	67	2024	0.54	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	108.00%		
8) Toluene-d8	7.33	98	5211	0.48	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.00%		
10) 1,1,2,2-Tetrachloroethane-	10.23	84	1053	0.52	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	104.00%		
Target Compounds						
3) Vinyl chloride	1.32	62	159m	0.025	ug/L	
6) Trichloroethene	5.95	95	90	0.024	ug/L #	83
9) 1,2-Dibromoethane	8.38	107	45	0.021	ug/L #	76
12) 1,2,3-Trichloropropane	10.28	75	40	0.023	ug/L #	58
13) 1,2-Dibromo-3-chloropropan	12.43	75	8m	0.029	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111920\
Data File : VV019406.D
Acq On : 19 Nov 2020 13:50
Operator : SY/MD
Sample : L4485-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-05

Manual Integrations
APPROVED

MMDadoda
11/30/2020 3:40:10 PM

Quant Time: Nov 20 11:18:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 20 00:26:09 2020
Response via : Initial Calibration

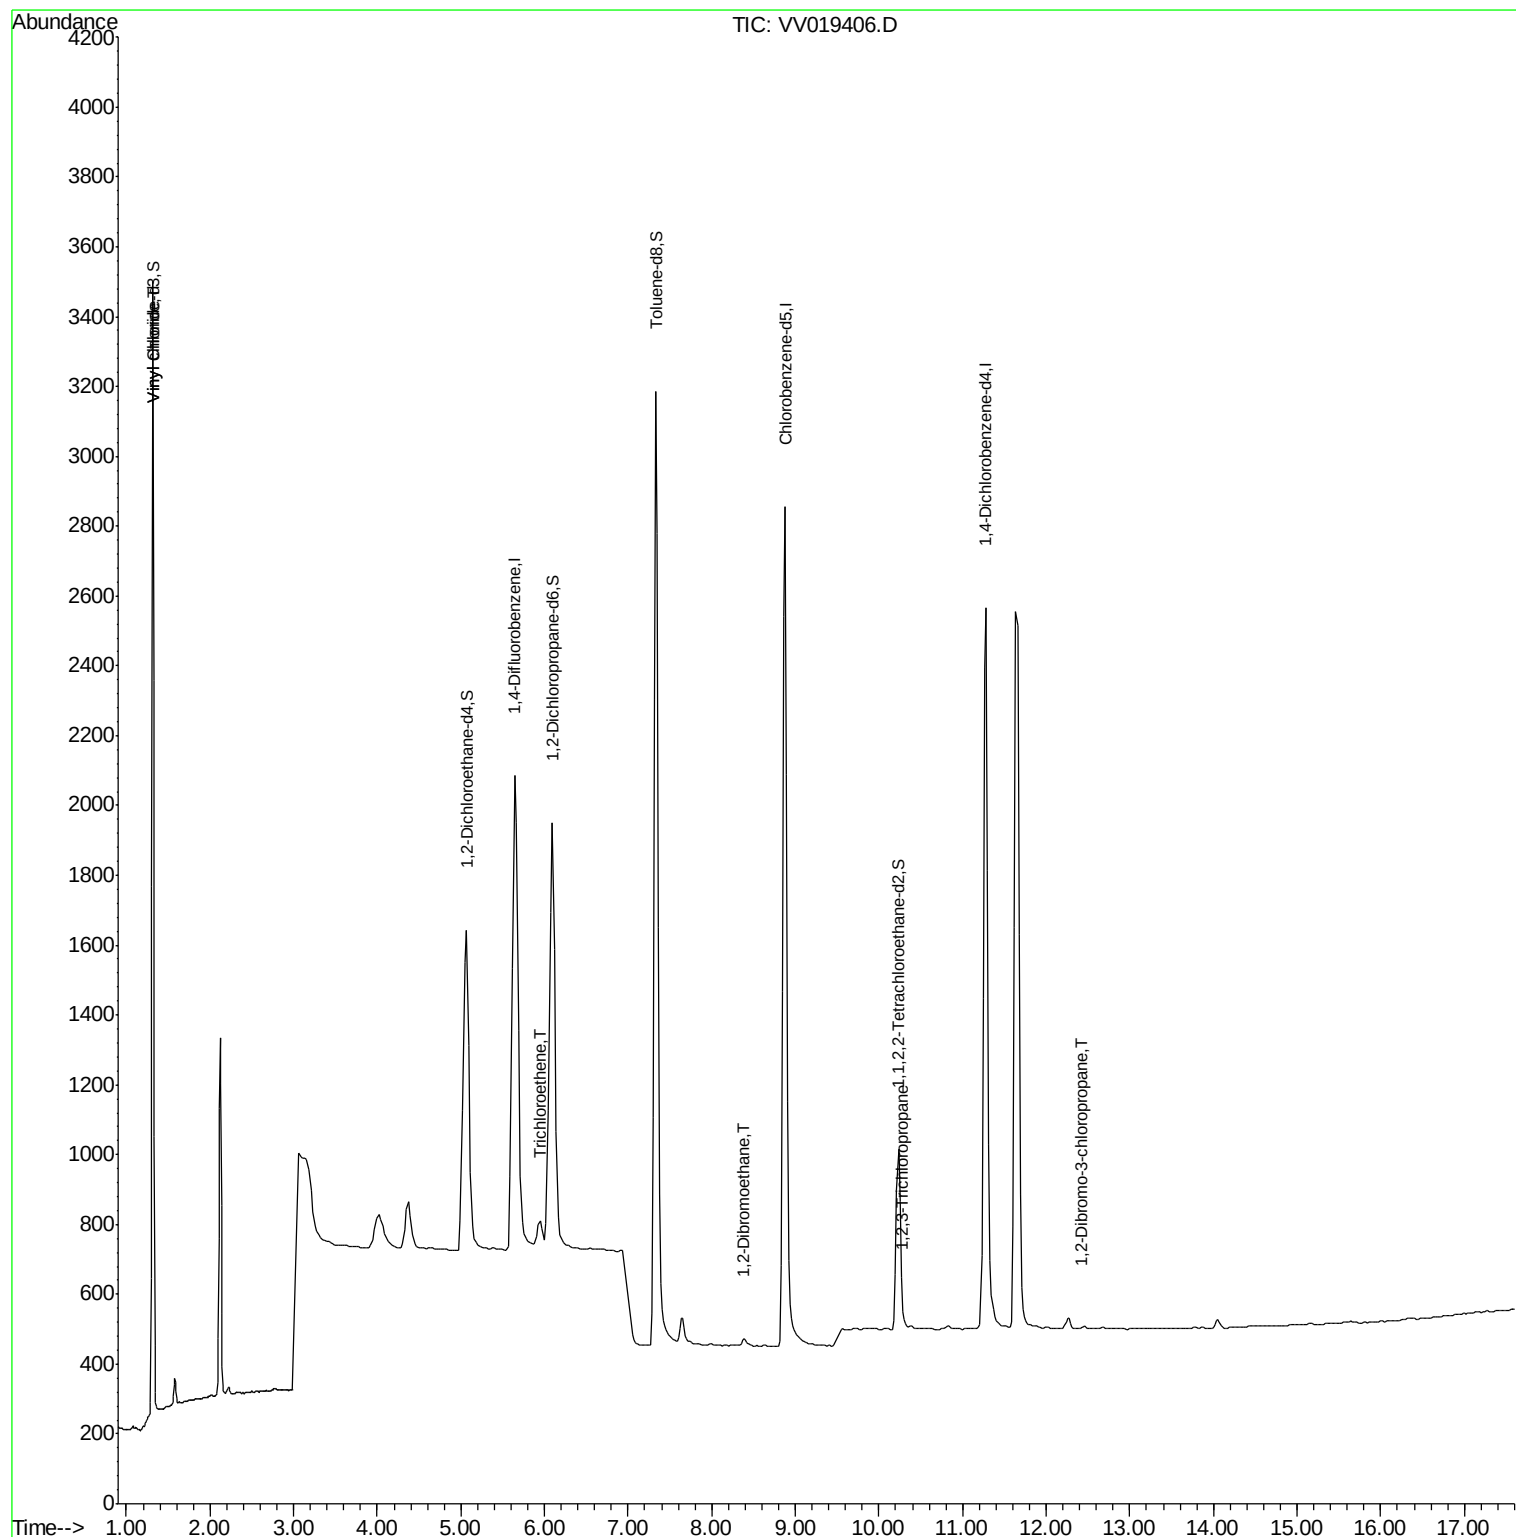

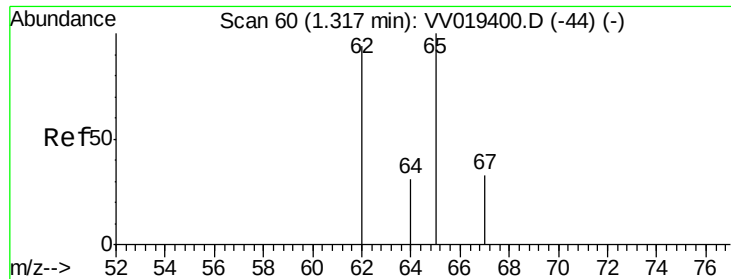

#3

Vinyl chloride

Concen: 0.025 ug/L m

RT: 1.32 min Scan# 60

Delta R.T. 0.00 min

Lab File: VV019406.D

Acq: 19 Nov 2020 13:50

Instrument :

MSVOA_V

ClientSampleId :

MDL-WATER-05

Tot Ion: 62 Resp: 159

Ion Ratio Lower Upper

62 100





64 85.4 25.1 46.7#

Manual Integrations

APPROVED

MMDadoda

11/30/2020 3:40:10 PM

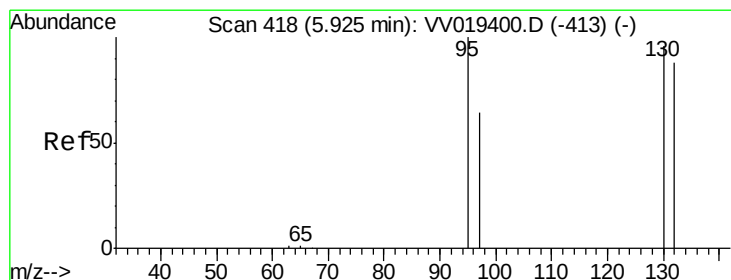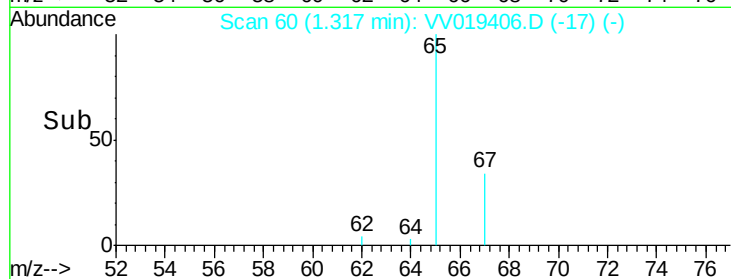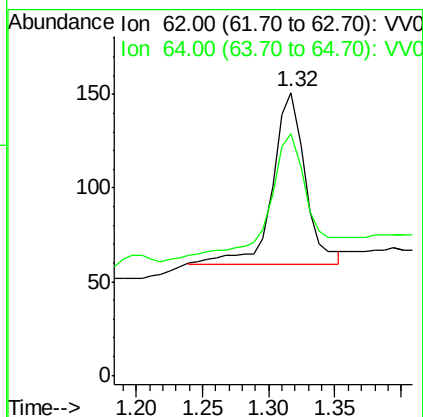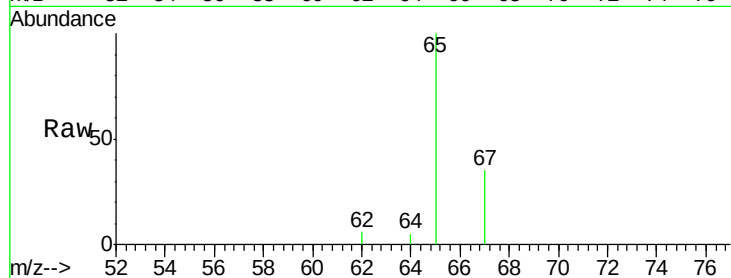

#6

Trichloroethene

Concen: 0.024 ug/L

RT: 5.95 min Scan# 419

Delta R.T. 0.02 min

Lab File: VV019406.D

Acq: 19 Nov 2020 13:50

Tgt Ion: 95 Resp: 90




Ion Ratio Lower Upper




95 100

97 91.3 45.6 84.6#

132 100.0 61.0 113.2

130 101.4 65.9 122.3

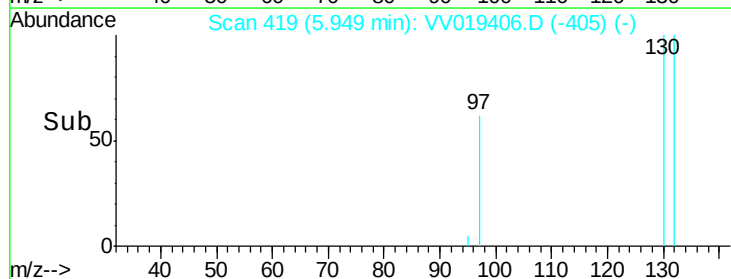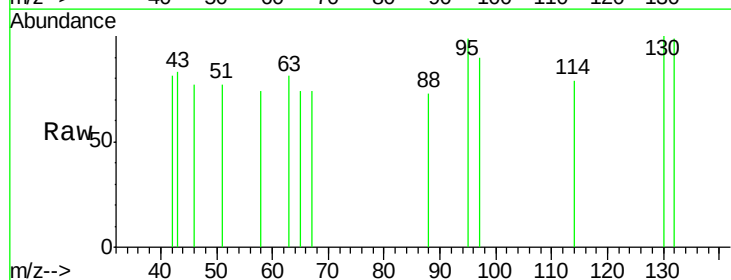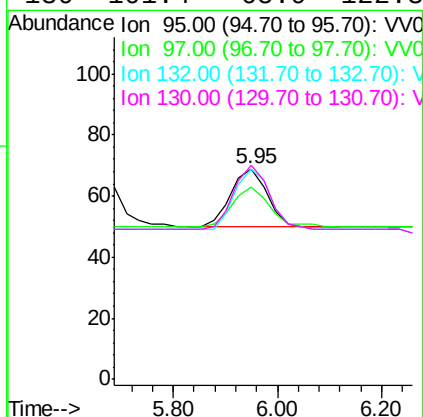

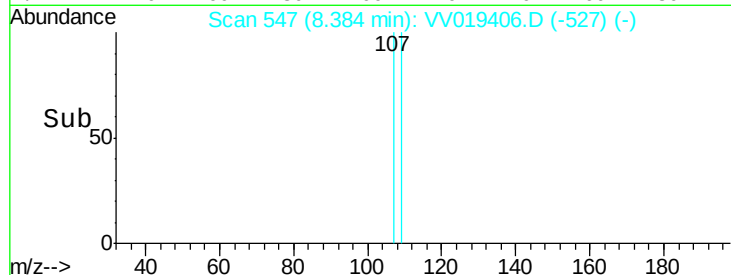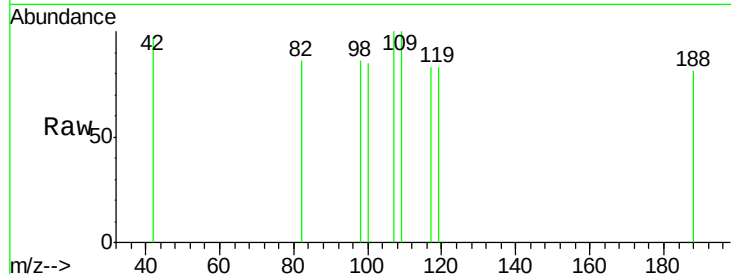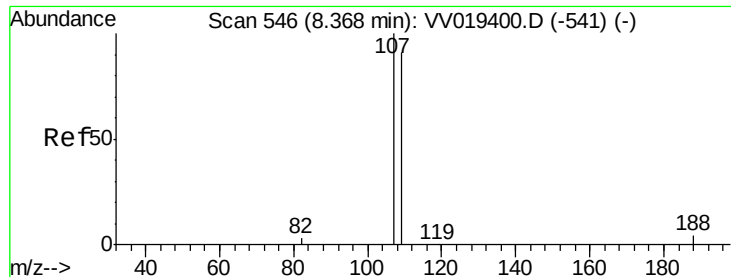





#9
 1,2-Dibromoethane
 Concen: 0.021 ug/L
 RT: 8.38 min Scan# 547
 Delta R.T. 0.02 min
 Lab File: VV019406.D
 Acq: 19 Nov 2020 13:50

Tot Ion	Ratio	Resp	Lower	Upper
107	100			
109	100.0	68.5	127.1	
188	81.4	13.9	20.9	

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-05


Manual Integrations
 APPROVED


MMDadoda
 11/30/2020 3:40:10 PM

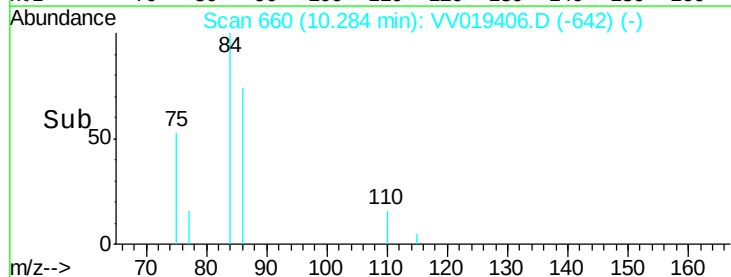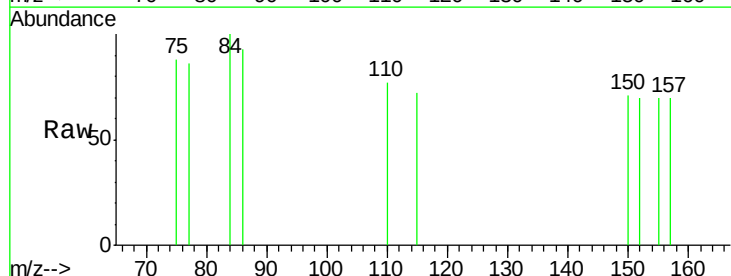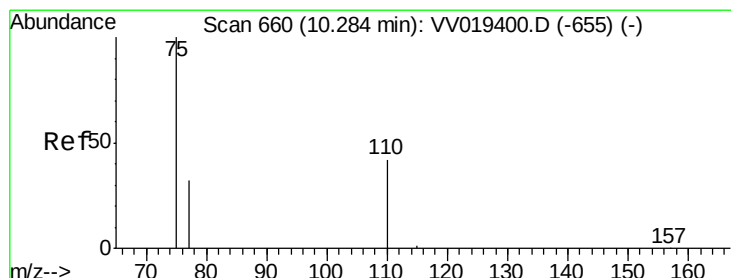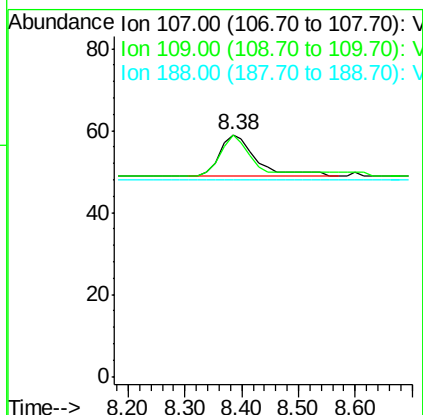

#12
 1,2,3-Trichloropropane
 Concen: 0.023 ug/L
 RT: 10.28 min Scan# 660
 Delta R.T. 0.00 min
 Lab File: VV019406.D
 Acq: 19 Nov 2020 13:50

Tgt Ion	Ratio	Resp	Lower	Upper
75	100			
110	0.0	34.5	51.7	
77	27.5	25.7	38.5	

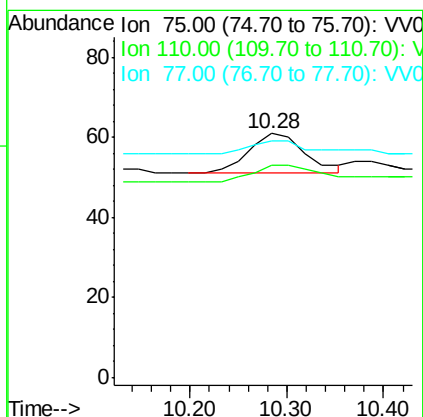

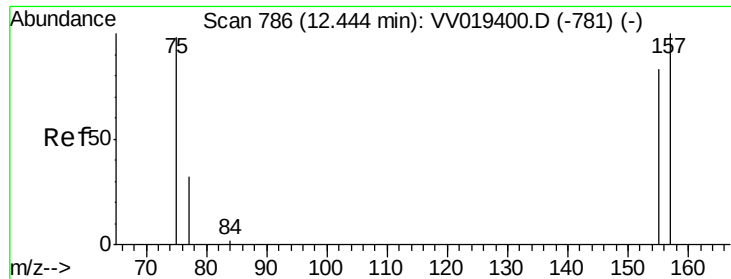

#13

1,2-Dibromo-3-chloropropane

Concen: 0.029 ug/L m

RT: 12.43 min Scan# 785

Delta R.T. -0.02 min

Lab File: VV019406.D

Acq: 19 Nov 2020 13:50

Instrument :

MSVOA_V

ClientSampleId :

MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
75	100		
157	92.5	79.2	118.8
155	92.5	71.0	106.6

Manual Integrations
APPROVED

MMDadoda
11/30/2020 3:40:10 PM

