


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111921\  
Data File : VV023648.D  
Acq On : 19 Nov 2021 17:03  
Operator : SY/MD  
Sample : M4706-21  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
B0AC0

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:49:49 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Mon Nov 22 01:44:25 2021  
Response via : Initial Calibration

Reviewed By :John Carlone 11/22/2021  
Supervised By :Mahesh Dadoda 11/22/2021

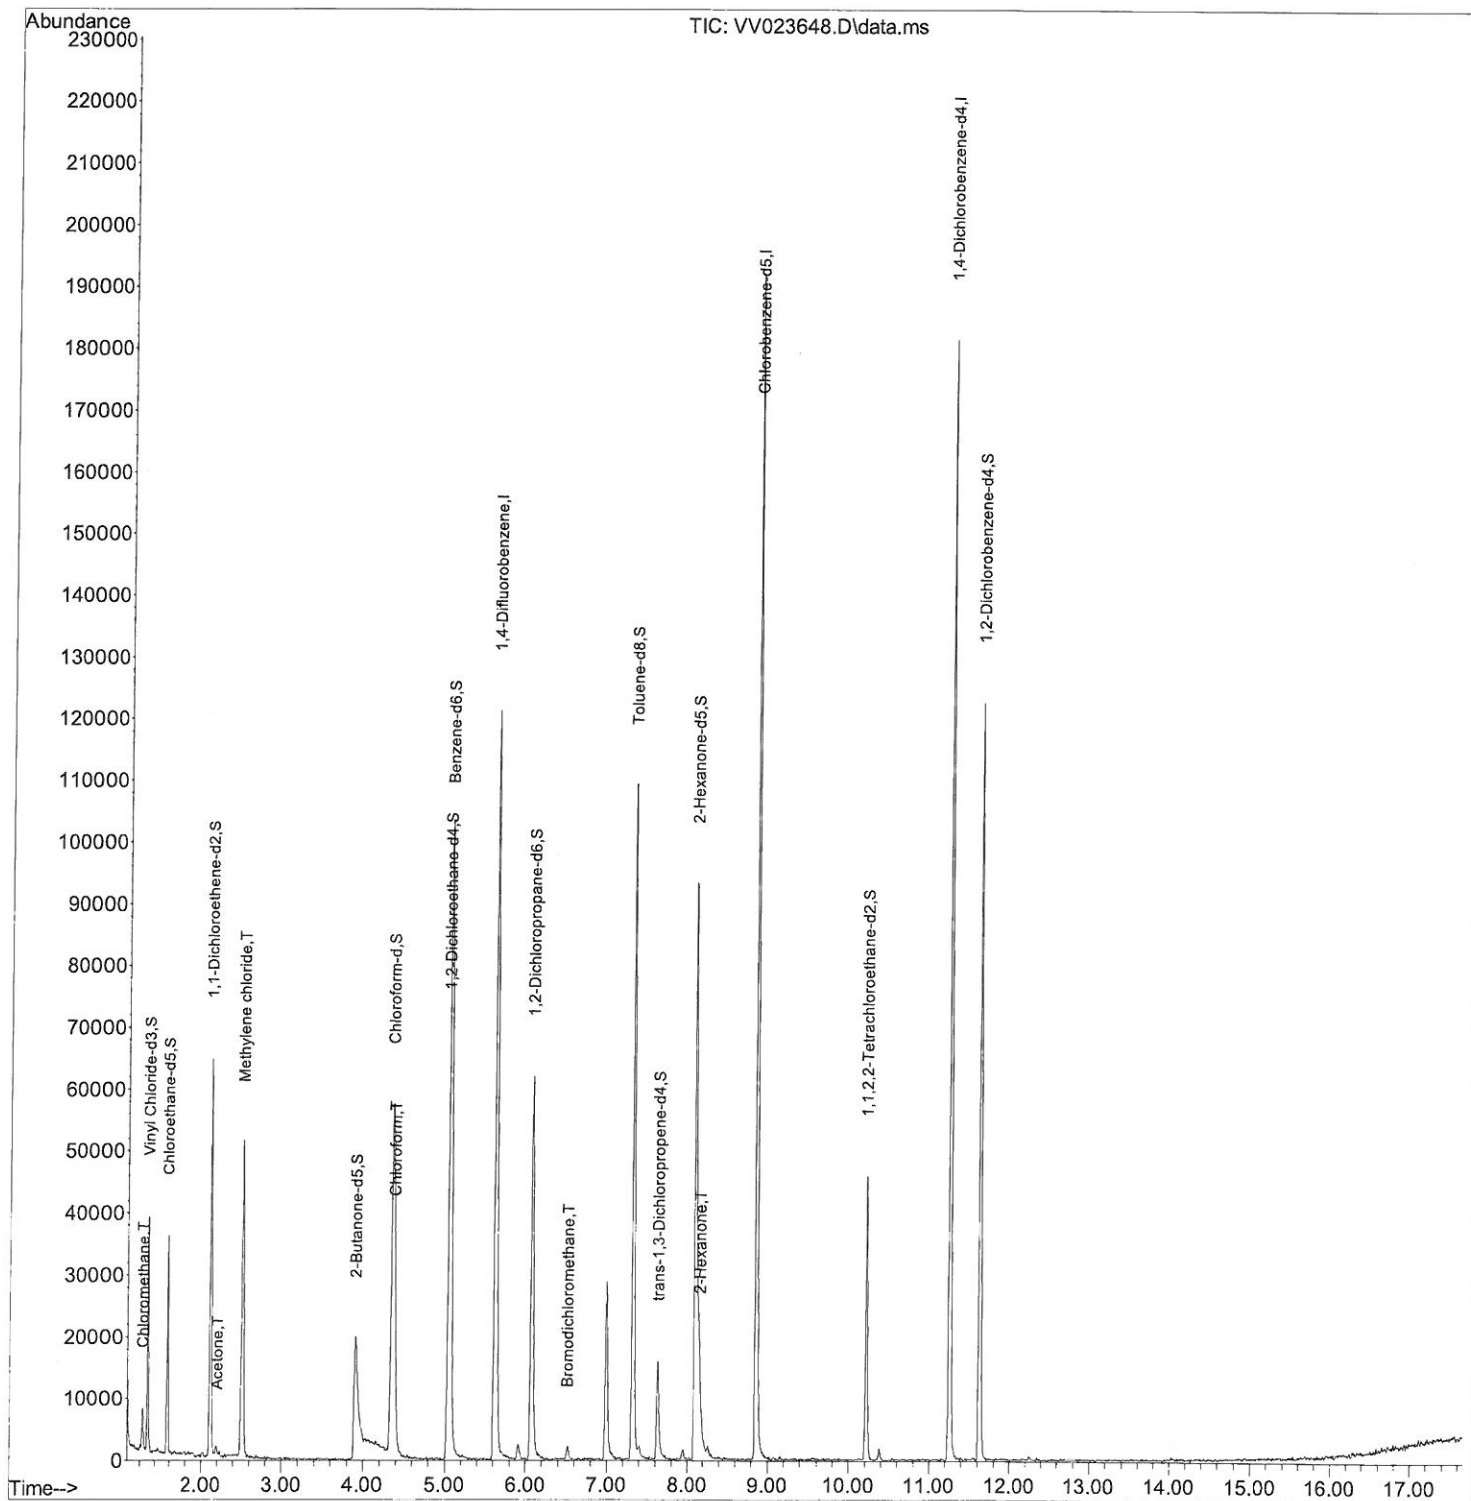

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111921\  
 Data File : VV023648.D  
 Acq On : 19 Nov 2021 17:03  
 Operator : SY/MD  
 Sample : M4706-21  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 B0AC0

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:49:49 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Mon Nov 22 01:44:25 2021  
 Response via : Initial Calibration

Reviewed By :John Carlone 11/22/2021  
 Supervised By :Mahesh Dadoda 11/22/2021

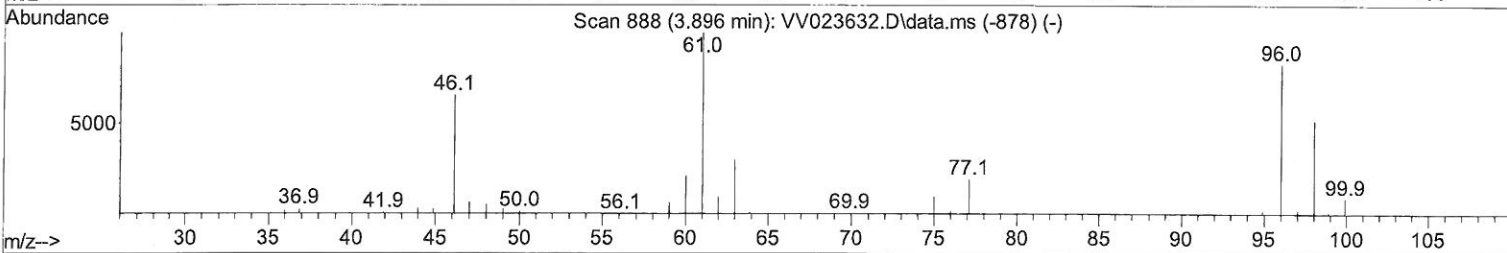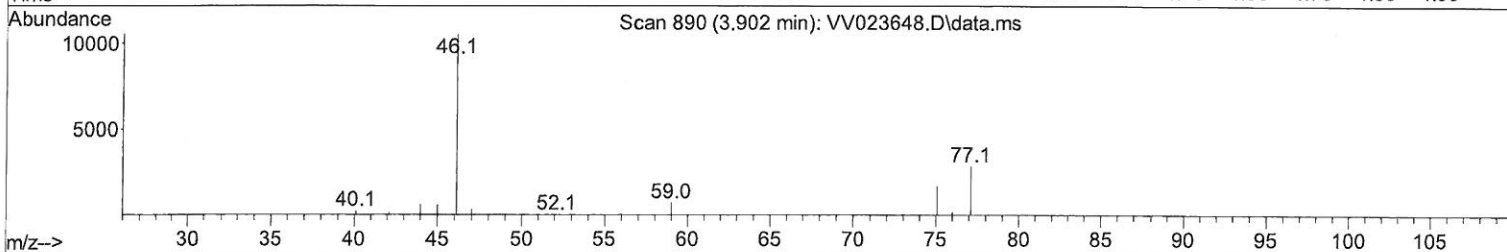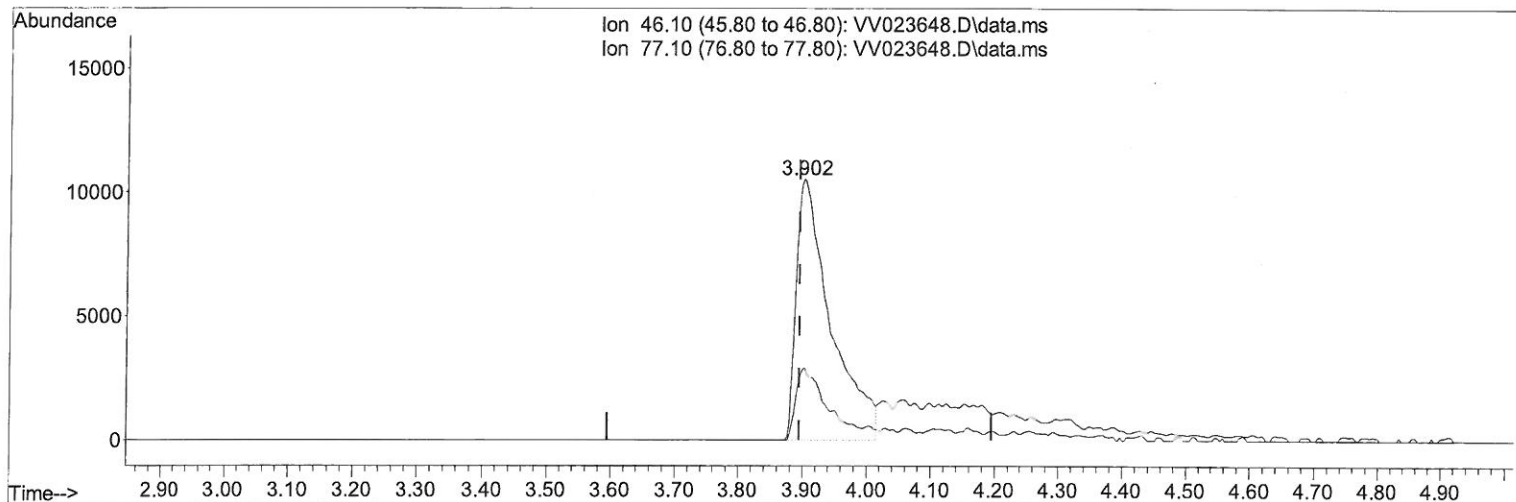

TIC: VV023648.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (+ 0.006) 33.17 ug/L

response 39133

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	25.19
0.00	0.00	0.00
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111921\  
 Data File : VV023648.D  
 Acq On : 19 Nov 2021 17:03  
 Operator : SY/MD  
 Sample : M4706-21  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 B0AC0

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:49:49 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Mon Nov 22 01:44:25 2021  
 Response via : Initial Calibration

Reviewed By :John Carlone 11/22/2021  
 Supervised By :Mahesh Dadoda 11/22/2021

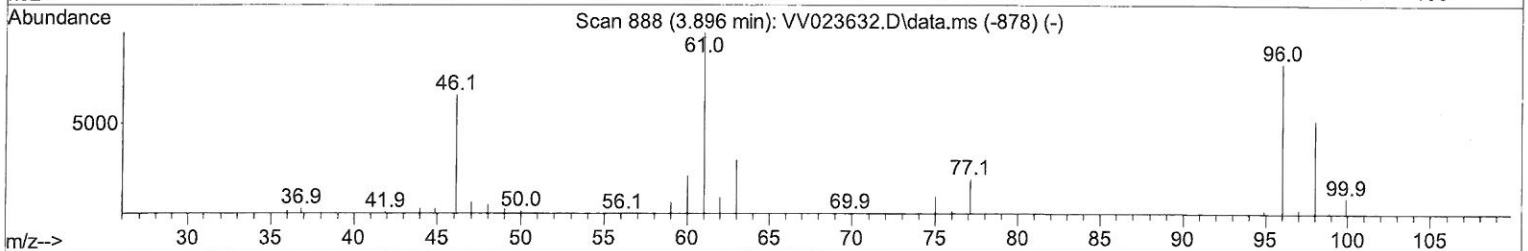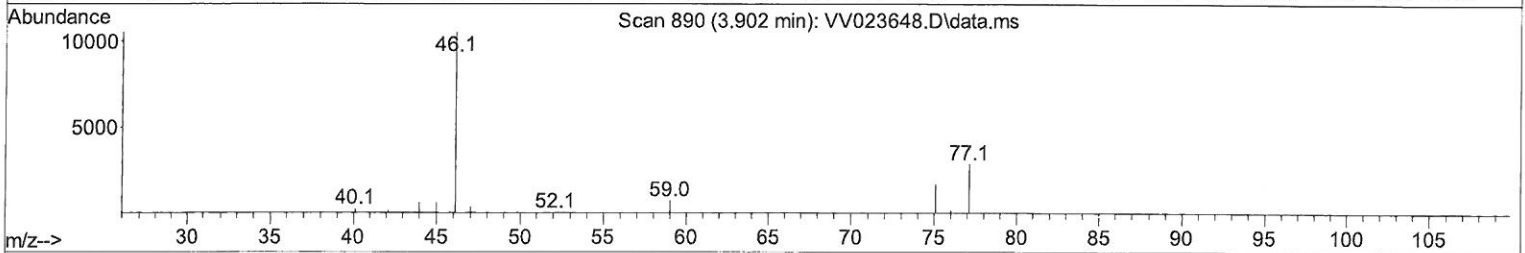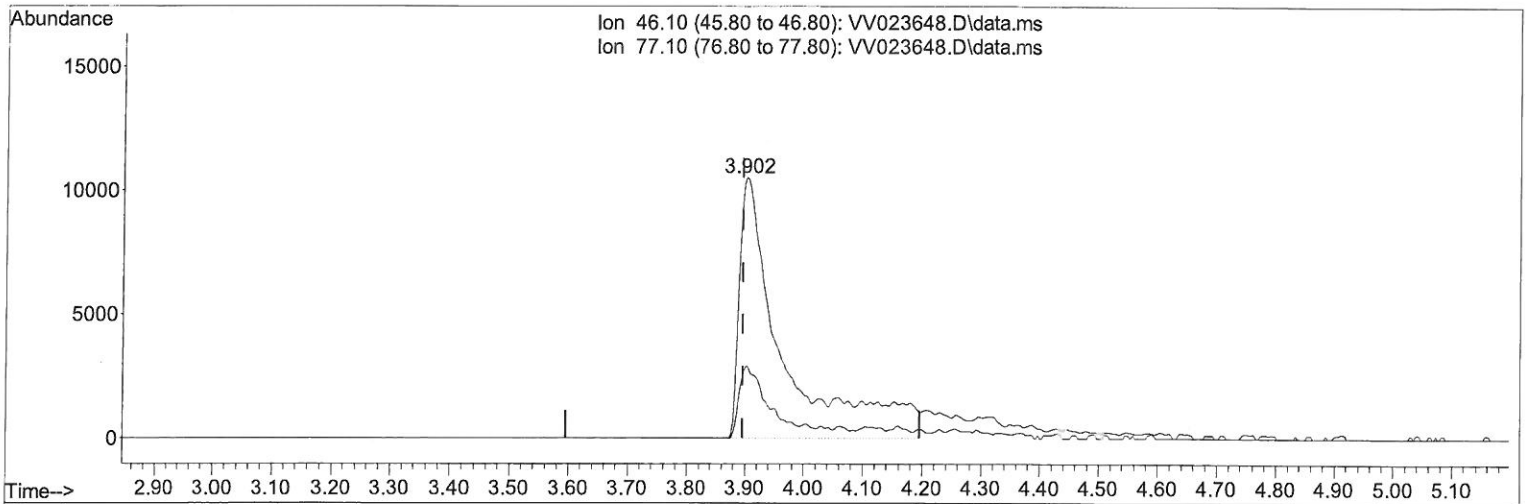

TIC: VV023648.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (+ 0.006) 46.16 ug/L m

response 54463

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	18.10
0.00	0.00	0.00
0.00	0.00	0.00

MD  
12/3/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111921\  
 Data File : VV023648.D  
 Acq On : 19 Nov 2021 17:03  
 Operator : SY/MD  
 Sample : M4706-21  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 B0AC0

## Manual IntegrationsAPPROVED

Reviewed By : John Carlone 11/22/2021  
 Supervised By : Mahesh Dadoda 11/22/2021

Quant Time: Nov 22 01:49:49 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Mon Nov 22 01:44:25 2021  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	109322	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	108715	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	48270	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	23292	3.401	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	68.000%	
7) Chloroethane-d5	1.568	69	20862	3.738	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	74.800%	
11) 1,1-Dichloroethene-d2	2.108	63	32484	2.534	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	50.600%#	
20) 2-Butanone-d5	3.902	46	54463m	46.159	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	92.320%	
24) Chloroform-d	4.352	84	54850	3.758	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	75.200%	
26) 1,2-Dichloroethane-d4	5.034	65	26224	3.996	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	80.000%	
32) Benzene-d6	5.053	84	91670	3.286	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	65.800%#	
36) 1,2-Dichloropropane-d6	6.072	67	29068	3.540	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	70.800%	
41) Toluene-d8	7.320	98	75376	2.884	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	57.600%#	
43) trans-1,3-Dichloroprop...	7.628	79	10478	3.365	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	67.400%	
46) 2-Hexanone-d5	8.091	63	39610	34.577	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	69.160%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	21987	3.723	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	74.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	32610	4.057	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	81.200%	
Target Compounds						Qvalue
3) Chloromethane	1.240	50	4388	0.484	ug/L	93
13) Acetone	2.198	43	2895	4.016	ug/L	98
16) Methylene chloride	2.510	84	21876	2.299	ug/L	97
25) Chloroform	4.378	83	18703	1.297	ug/L	94
38) Bromodichloromethane	6.516	83	1727	0.182	ug/L #	85
48) 2-Hexanone	8.152	43	5106	2.215	ug/L #	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed