

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023635.D
 Acq On : 19 Nov 2021 11:54
 Operator : SY/MD
 Sample : M4706-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	55	62	74	rBV	5512	6975	2.09%	0.237%
2	1.307	75	83	97	rVB	50135	52885	15.85%	1.795%
3	1.568	155	164	177	rBV	46601	51756	15.51%	1.757%
4	2.108	321	332	349	rBV	87538	126271	37.84%	4.287%
5	2.506	446	456	476	rVB	47229	80192	24.03%	2.723%
6	3.908	878	892	921	rBV3	17898	71393	21.40%	2.424%
7	4.352	1014	1030	1064	rVB3	65376	200350	60.04%	6.802%
8	5.050	1231	1247	1270	rBV3	132018	330516	99.05%	11.221%
9	5.619	1410	1424	1449	rBV	130581	265206	79.48%	9.004%
10	6.072	1551	1565	1588	rBV	76241	157369	47.16%	5.343%
11	6.519	1694	1704	1714	rBV5	2335	4128	1.24%	0.140%
12	6.989	1834	1850	1869	rBV	36507	68673	20.58%	2.331%
13	7.317	1936	1952	1974	rBV	148974	265991	79.71%	9.031%
14	7.625	2040	2048	2067	rBV	20624	39031	11.70%	1.325%
15	7.937	2136	2145	2157	rBV3	2783	4940	1.48%	0.168%
16	8.095	2184	2194	2231	rBV	102344	263772	79.05%	8.955%
17	8.853	2418	2430	2449	rBV	203251	333685	100.00%	11.329%
18	10.217	2844	2854	2869	rBV	50349	82769	24.80%	2.810%
19	10.384	2894	2906	2916	rBV3	3578	5727	1.72%	0.194%
20	11.249	3164	3175	3199	rBV	194133	298409	89.43%	10.131%
21	11.625	3281	3292	3313	rBV	150199	235421	70.55%	7.993%




Sum of corrected areas: 2945459

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023635.D
Acq On : 19 Nov 2021 11:54
Operator : SY/MD
Sample : M4706-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

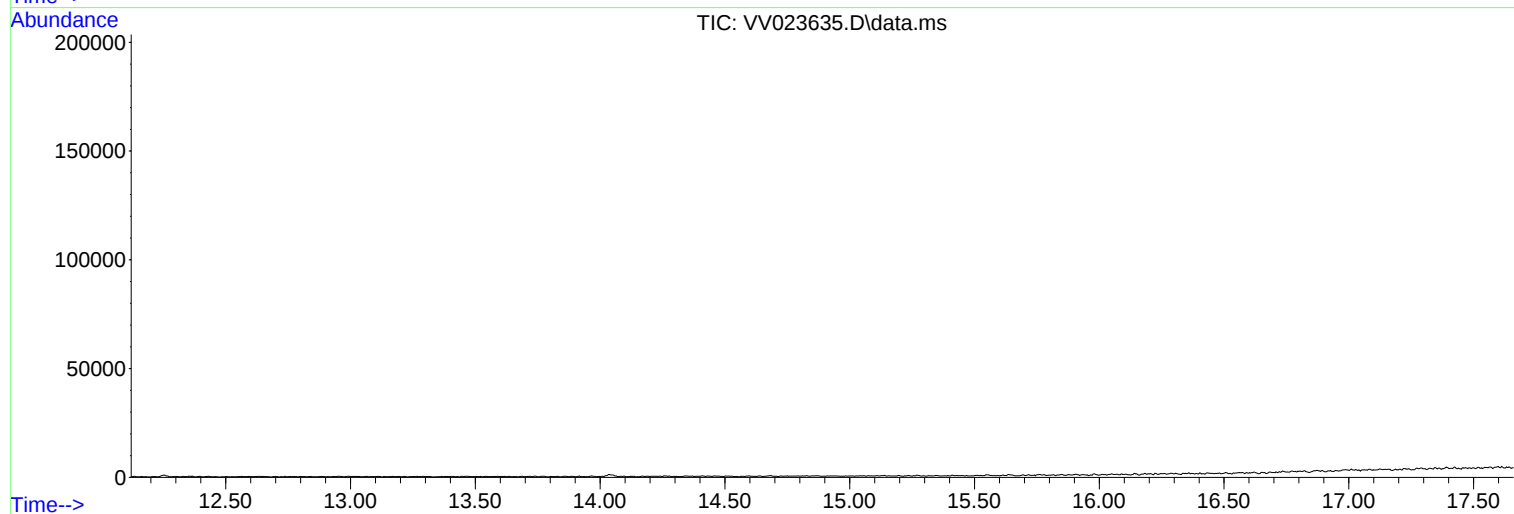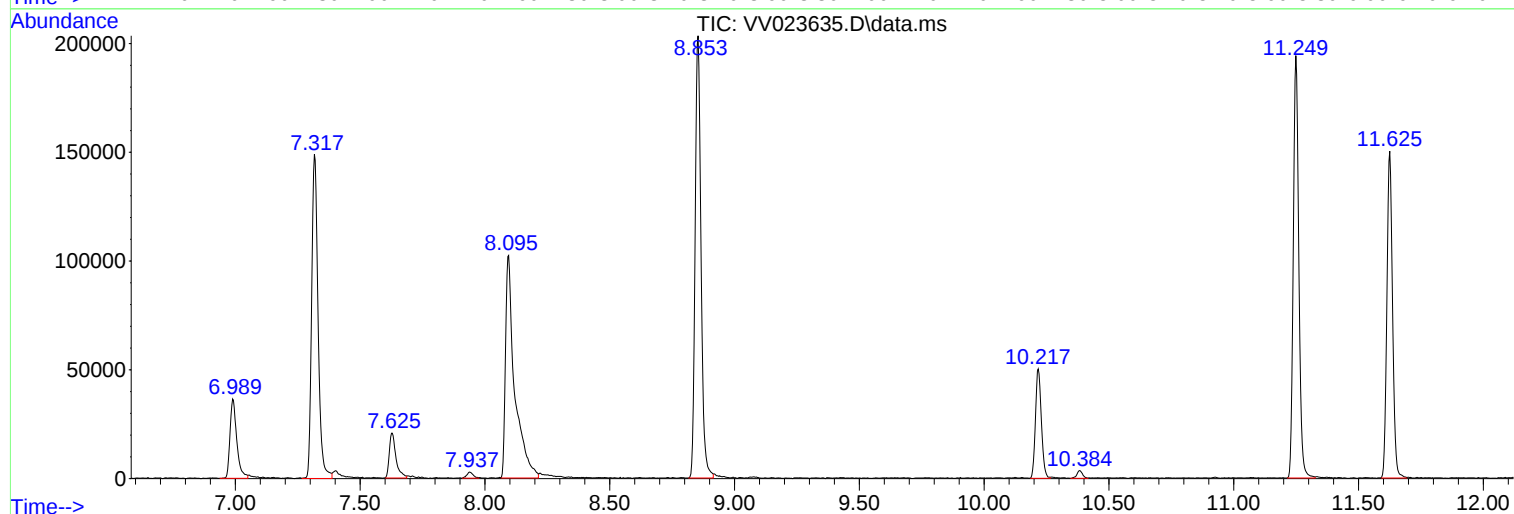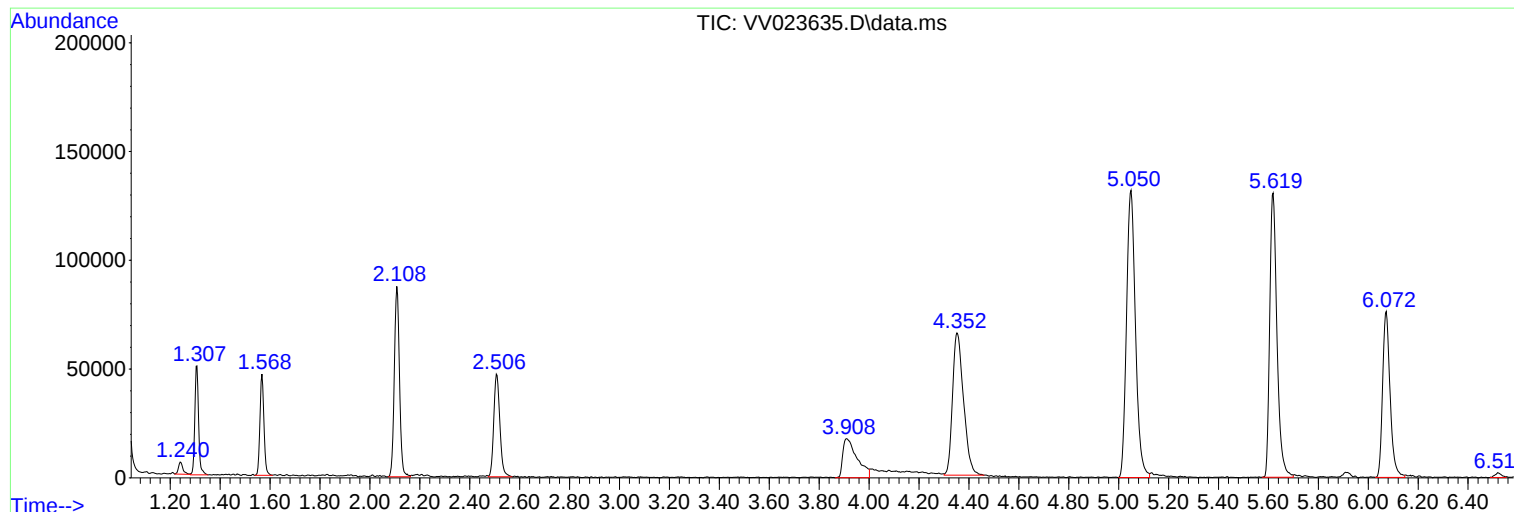

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023635.D
Acq On : 19 Nov 2021 11:54
Operator : SY/MD
Sample : M4706-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023635.D
Acq On : 19 Nov 2021 11:54
Operator : SY/MD
Sample : M4706-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc