

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023637.D
 Acq On : 19 Nov 2021 12:41
 Operator : SY/MD
 Sample : M4706-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	56	62	70	rVB2	4802	5441	1.65%	0.188%
2	1.304	76	82	95	rVB	49302	50811	15.42%	1.758%
3	1.568	156	164	174	rBV	44258	50734	15.39%	1.755%
4	2.108	321	332	345	rBV	87885	123635	37.51%	4.278%
5	2.507	445	456	480	rVB	56912	96070	29.15%	3.324%
6	3.905	879	891	921	rBV3	18839	71511	21.70%	2.474%
7	4.352	1012	1030	1051	rBV4	65957	195288	59.25%	6.757%
8	5.050	1231	1247	1274	rBV3	131942	329584	100.00%	11.404%
9	5.619	1411	1424	1447	rBV	124501	254062	77.09%	8.791%
10	5.912	1507	1515	1525	rBV5	2482	4805	1.46%	0.166%
11	6.072	1550	1565	1585	rBV2	74468	155901	47.30%	5.394%
12	6.519	1695	1704	1716	rVB5	2291	4225	1.28%	0.146%
13	6.989	1839	1850	1866	rBV2	34439	65104	19.75%	2.253%
14	7.317	1941	1952	1971	rBV	148687	263041	79.81%	9.102%
15	7.629	2039	2049	2068	rBV2	20307	38444	11.66%	1.330%
16	8.092	2184	2193	2232	rBV	98767	259604	78.77%	8.983%
17	8.854	2418	2430	2458	rBV	192818	321215	97.46%	11.114%
18	10.217	2843	2854	2870	rBV	51052	82962	25.17%	2.871%
19	10.384	2898	2906	2919	rVB4	2679	4065	1.23%	0.141%
20	11.249	3165	3175	3199	rBV	180947	280514	85.11%	9.706%
21	11.625	3281	3292	3312	rBV	147417	233064	70.71%	8.064%




Sum of corrected areas: 2890080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023637.D
Acq On : 19 Nov 2021 12:41
Operator : SY/MD
Sample : M4706-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

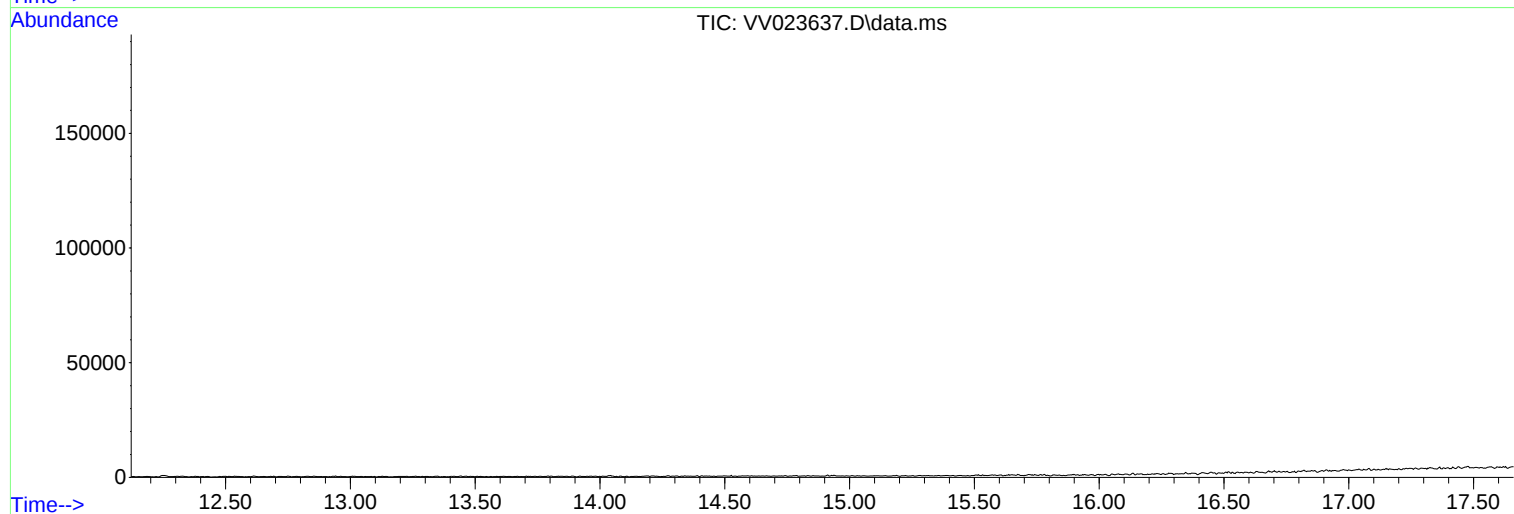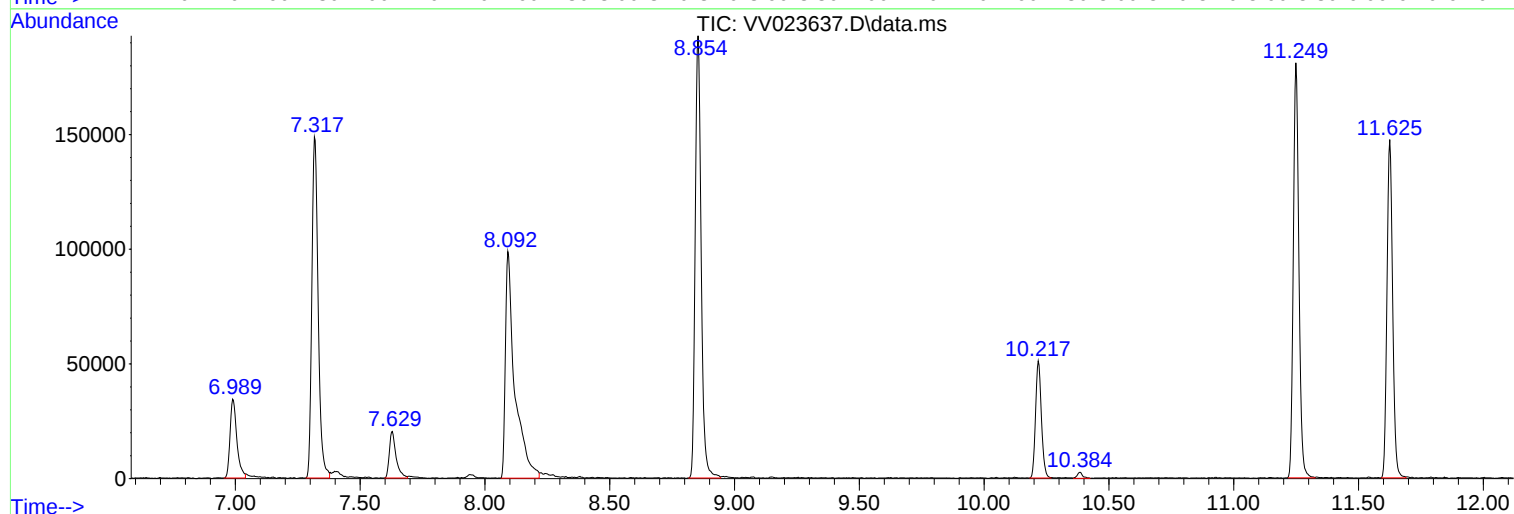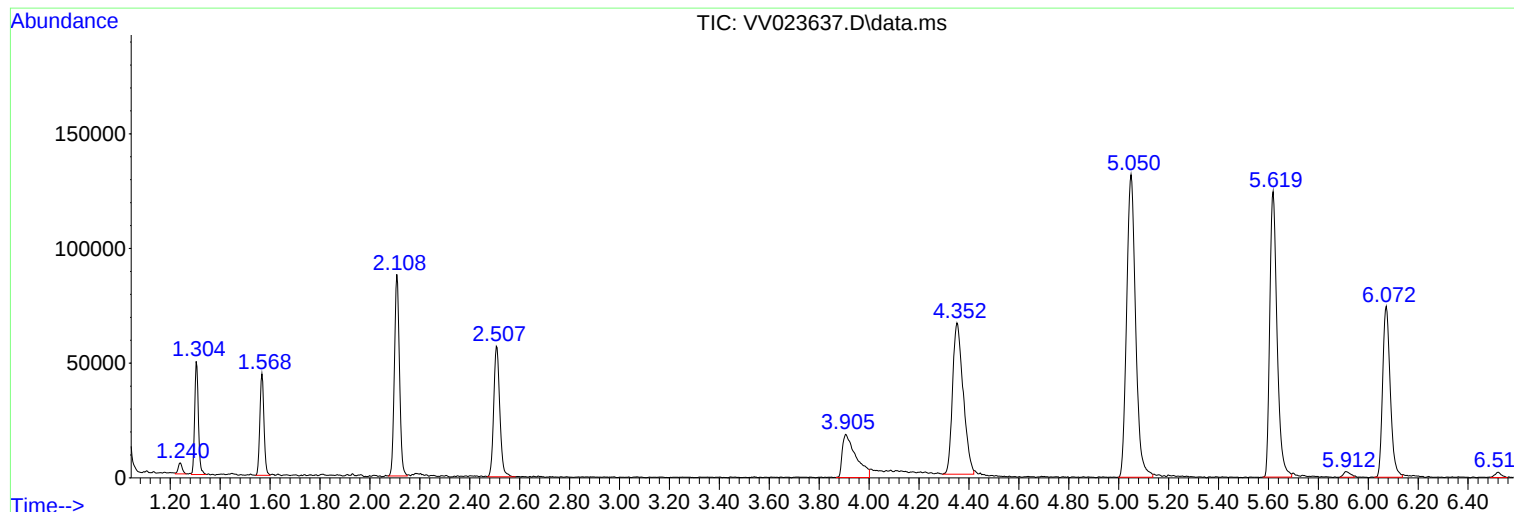

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023637.D
Acq On : 19 Nov 2021 12:41
Operator : SY/MD
Sample : M4706-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023637.D
Acq On : 19 Nov 2021 12:41
Operator : SY/MD
Sample : M4706-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc