

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023638.D
 Acq On : 19 Nov 2021 13:05
 Operator : SY/MD
 Sample : M4706-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AB8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	51700	53200	16.11%	1.844%
2	1.568	155	164	172	rBV	46322	52261	15.82%	1.812%
3	2.108	322	332	347	rBV	86260	125394	37.96%	4.347%
4	2.506	445	456	475	rVB2	58779	95739	28.98%	3.319%
5	3.908	878	892	917	rBV3	18454	70091	21.22%	2.430%
6	4.346	1013	1028	1061	rVB3	65159	197909	59.91%	6.862%
7	5.046	1230	1246	1270	rBV2	131189	330324	100.00%	11.452%
8	5.616	1411	1423	1447	rBV	119053	249029	75.39%	8.634%
9	5.915	1506	1516	1527	rBV6	2855	5265	1.59%	0.183%
10	6.069	1551	1564	1586	rBV2	75373	156875	47.49%	5.439%
11	6.516	1696	1703	1713	rBV6	2615	4102	1.24%	0.142%
12	6.989	1840	1850	1865	rBV	34783	64782	19.61%	2.246%
13	7.316	1941	1952	1973	rBV	148094	264587	80.10%	9.173%
14	7.400	1973	1978	1988	rVB5	3018	5094	1.54%	0.177%
15	7.625	2037	2048	2063	rBV3	20087	37075	11.22%	1.285%
16	8.091	2182	2193	2232	rBV	100544	259748	78.63%	9.006%
17	8.853	2418	2430	2453	rBV	188588	313082	94.78%	10.855%
18	10.217	2842	2854	2876	rVB	52124	85861	25.99%	2.977%
19	10.377	2895	2904	2914	rBV3	2362	3387	1.03%	0.117%
20	11.249	3164	3175	3196	rBV	181320	278621	84.35%	9.660%
21	11.625	3281	3292	3312	rBV	144683	231893	70.20%	8.040%




Sum of corrected areas: 2884319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023638.D
Acq On : 19 Nov 2021 13:05
Operator : SY/MD
Sample : M4706-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

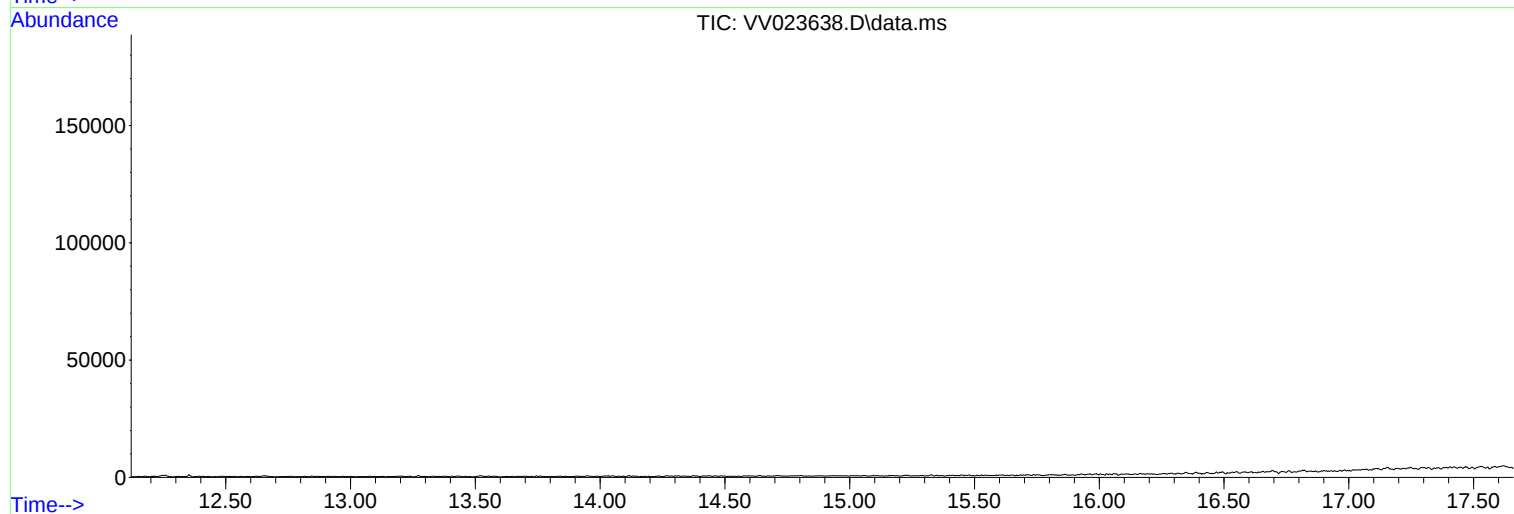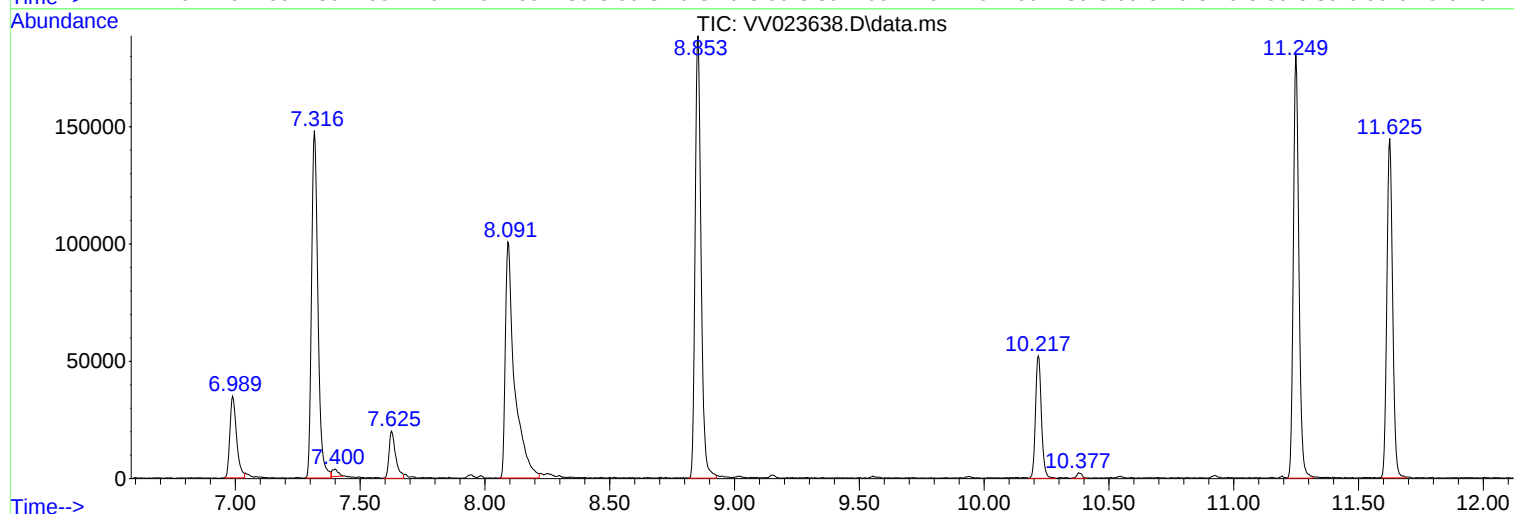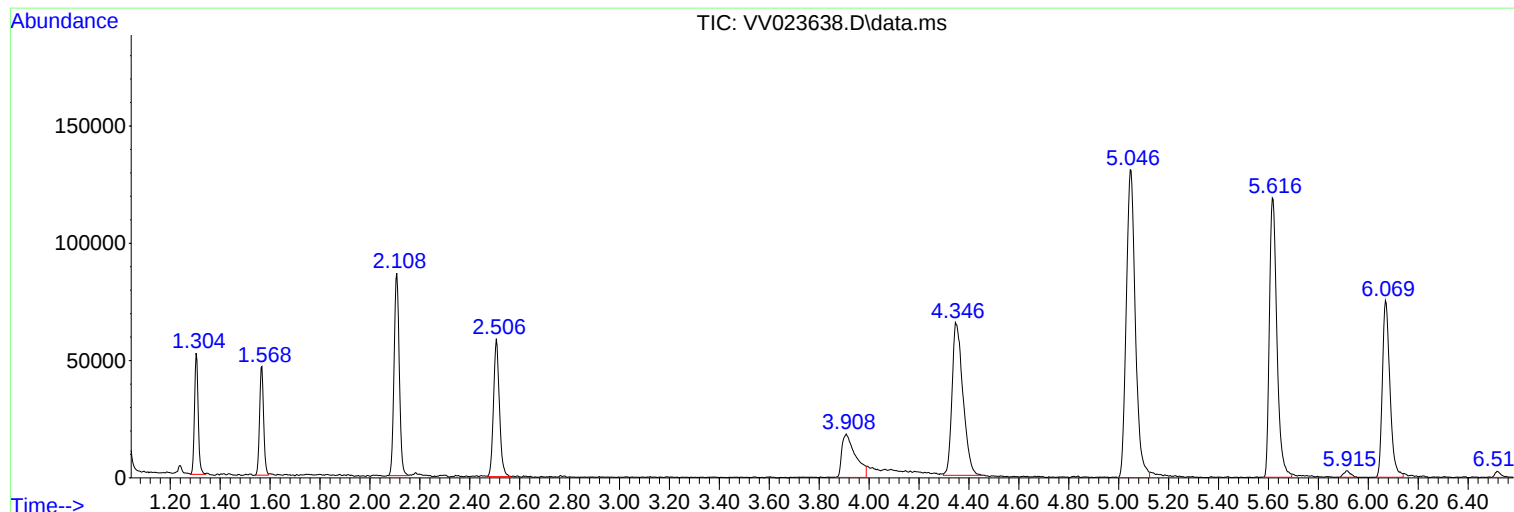

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023638.D
Acq On : 19 Nov 2021 13:05
Operator : SY/MD
Sample : M4706-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023638.D
Acq On : 19 Nov 2021 13:05
Operator : SY/MD
Sample : M4706-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc