

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023644.D
 Acq On : 19 Nov 2021 15:28
 Operator : SY/MD
 Sample : M4706-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	56	62	75	rVB	11693	13433	4.30%	0.496%
2	1.304	75	82	96	rVB	46891	49232	15.76%	1.817%
3	1.568	156	164	174	rBV	43084	48612	15.56%	1.794%
4	2.108	320	332	344	rBV	79897	115136	36.85%	4.249%
5	3.908	879	892	908	rBV2	21348	70943	22.71%	2.618%
6	4.352	1014	1030	1063	rVB4	64224	178301	57.07%	6.580%
7	5.050	1231	1247	1272	rBV3	124497	312436	100.00%	11.531%
8	5.619	1413	1424	1451	rBV	117613	241247	77.21%	8.904%
9	6.072	1552	1565	1589	rBV	72806	153313	49.07%	5.658%
10	6.519	1695	1704	1713	rBV4	3042	5544	1.77%	0.205%
11	6.989	1840	1850	1872	rBV	32929	63841	20.43%	2.356%
12	7.317	1940	1952	1969	rBV	138743	247076	79.08%	9.119%
13	7.625	2035	2048	2064	rBV2	19489	37137	11.89%	1.371%
14	7.976	2149	2157	2171	rVB3	16529	29031	9.29%	1.071%
15	8.095	2183	2194	2236	rBV	107825	270129	86.46%	9.969%
16	8.854	2419	2430	2451	rBV	183505	302317	96.76%	11.157%
17	10.217	2844	2854	2873	rBV2	51521	83768	26.81%	3.092%
18	11.249	3164	3175	3191	rBV	168275	263958	84.48%	9.742%
19	11.625	3281	3292	3313	rBV	141695	224116	71.73%	8.271%




Sum of corrected areas: 2709570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023644.D
Acq On : 19 Nov 2021 15:28
Operator : SY/MD
Sample : M4706-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

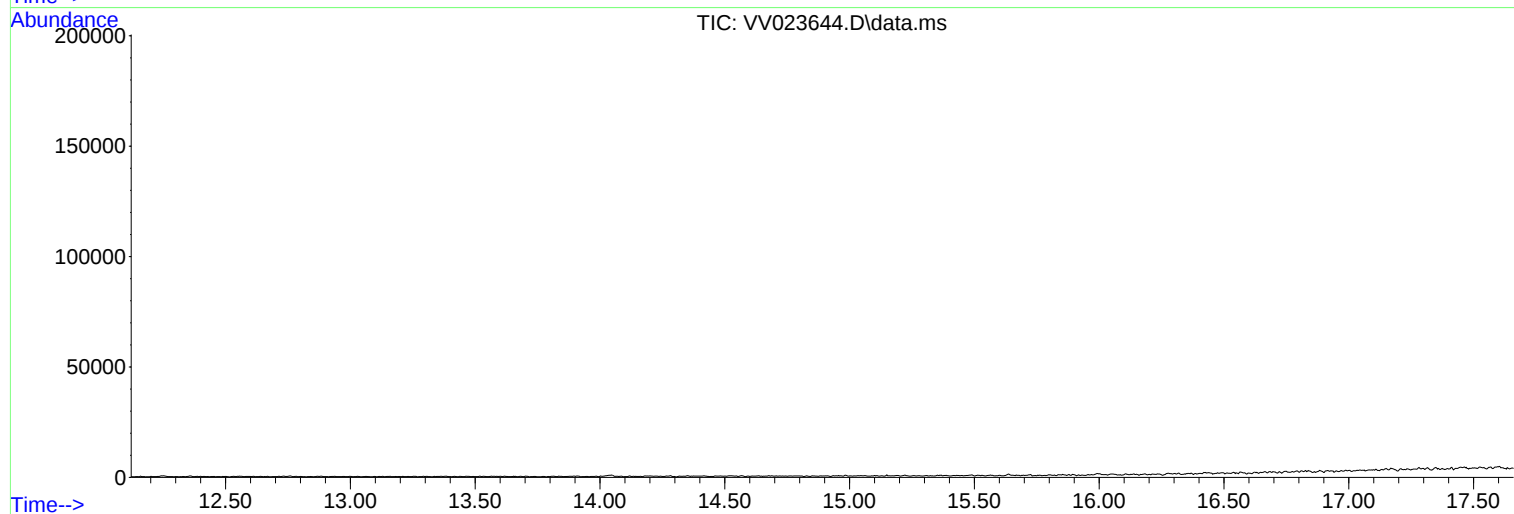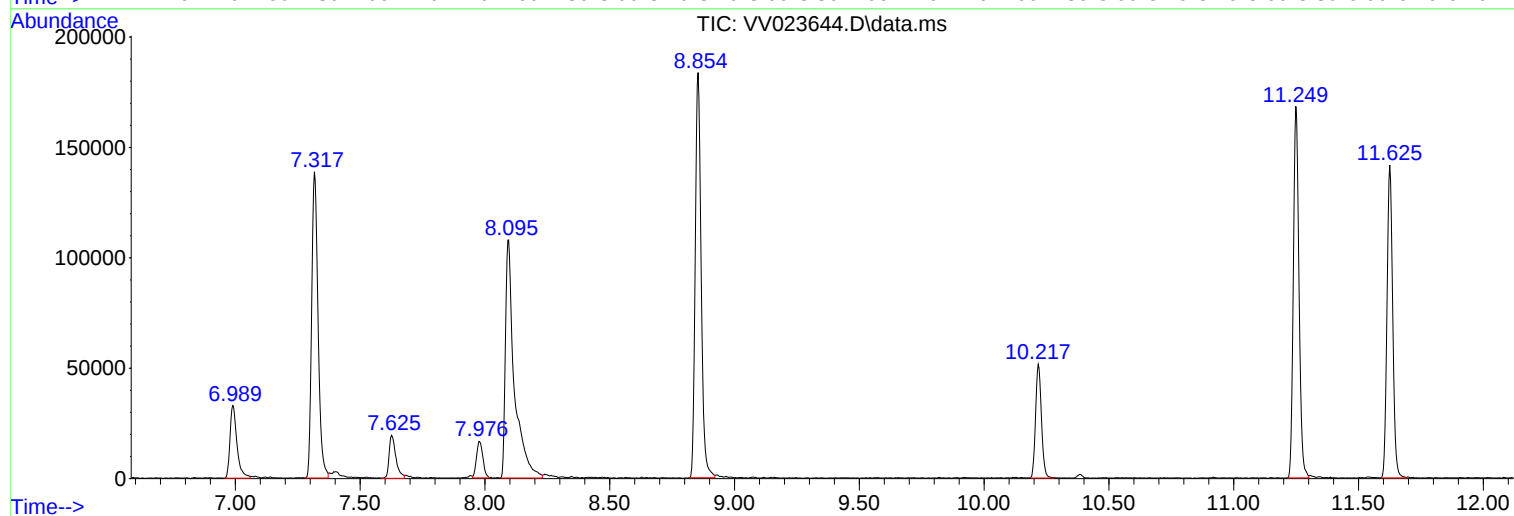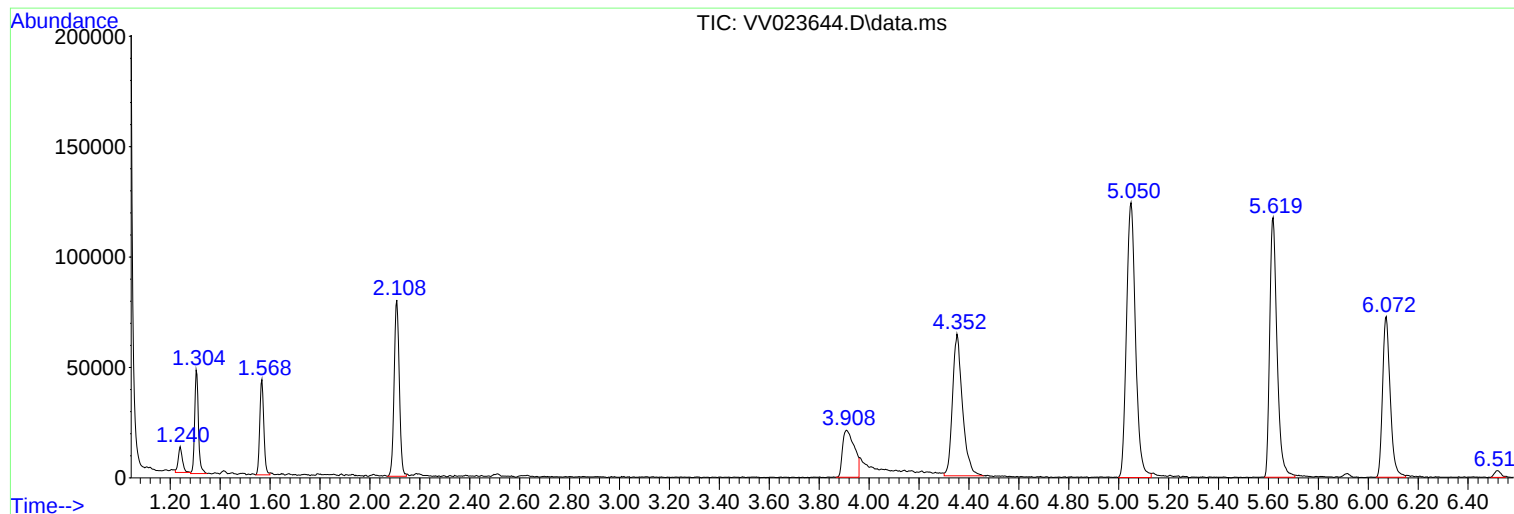

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023644.D
Acq On : 19 Nov 2021 15:28
Operator : SY/MD
Sample : M4706-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023644.D
Acq On : 19 Nov 2021 15:28
Operator : SY/MD
Sample : M4706-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc