

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023645.D
 Acq On : 19 Nov 2021 15:52
 Operator : SY/MD
 Sample : M4706-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	56	62	69	rVB2	7916	8996	2.92%	0.339%
2	1.304	75	82	97	rVB	44949	45738	14.86%	1.723%
3	1.568	155	164	173	rBV	41585	46565	15.13%	1.754%
4	2.108	321	332	345	rBV	75283	108840	35.35%	4.101%
5	3.915	882	894	924	rBV3	18051	78136	25.38%	2.944%
6	4.352	1015	1030	1055	rBV4	60151	175809	57.11%	6.624%
7	5.050	1228	1247	1268	rBV3	120601	299654	97.34%	11.290%
8	5.619	1412	1424	1444	rBV	119821	243941	79.24%	9.191%
9	5.911	1508	1515	1528	rVB5	1938	3631	1.18%	0.137%
10	6.072	1552	1565	1584	rBV	68813	144892	47.07%	5.459%
11	6.519	1692	1704	1716	rBV4	4131	7600	2.47%	0.286%
12	6.989	1840	1850	1872	rBV	31532	62307	20.24%	2.348%
13	7.317	1941	1952	1973	rBV	131181	231402	75.17%	8.719%
14	7.628	2039	2049	2066	rBV	18168	33733	10.96%	1.271%
15	7.979	2149	2158	2173	rVB3	13777	24432	7.94%	0.921%
16	8.095	2183	2194	2232	rBV	104710	262090	85.14%	9.875%
17	8.853	2417	2430	2449	rBV	188179	307850	100.00%	11.599%
18	10.217	2843	2854	2871	rBV	51784	83744	27.20%	3.155%
19	11.249	3164	3175	3194	rBV	176283	272536	88.53%	10.269%
20	11.625	3279	3292	3308	rBV	131900	212162	68.92%	7.994%




Sum of corrected areas: 2654058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023645.D
Acq On : 19 Nov 2021 15:52
Operator : SY/MD
Sample : M4706-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

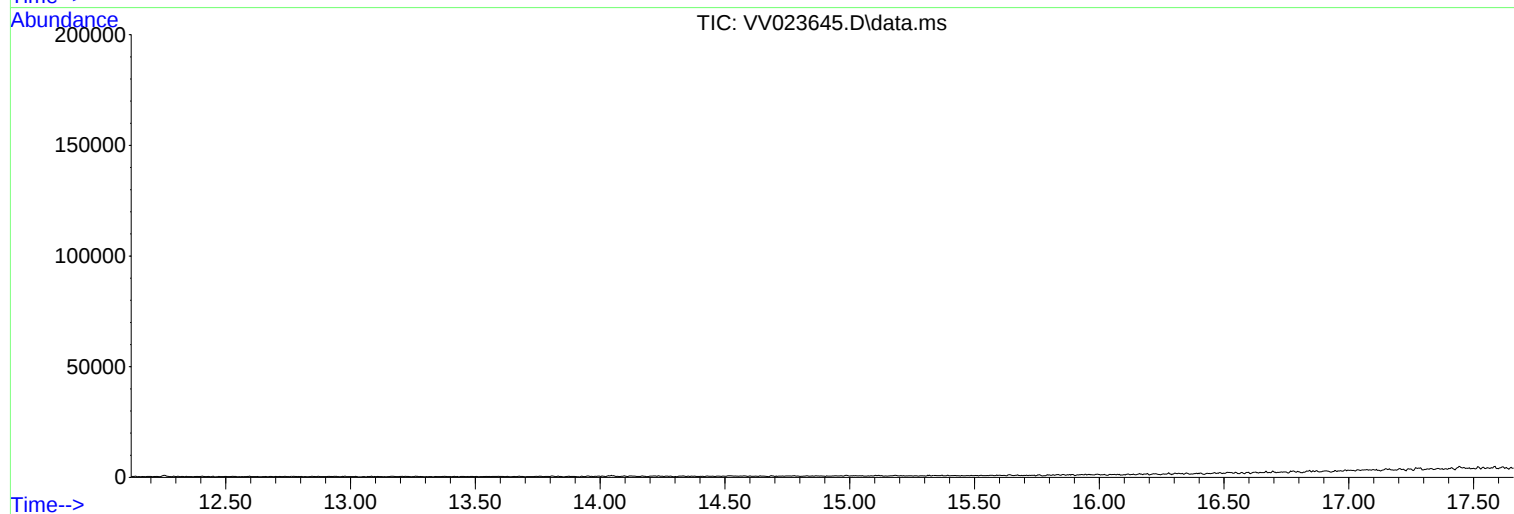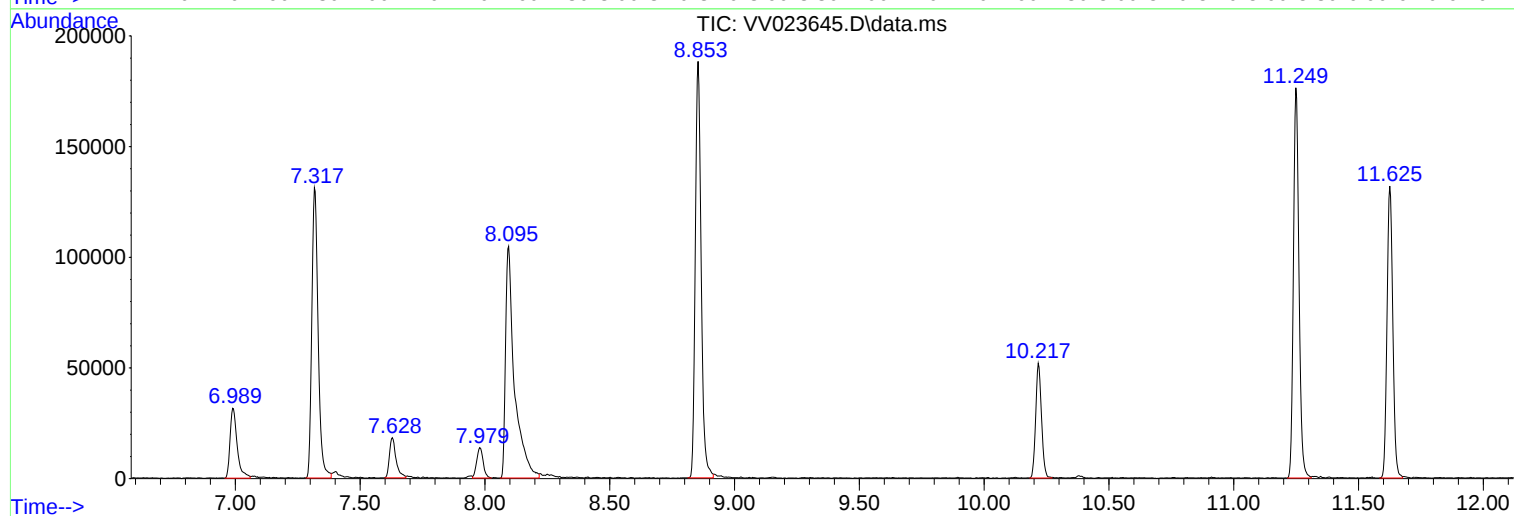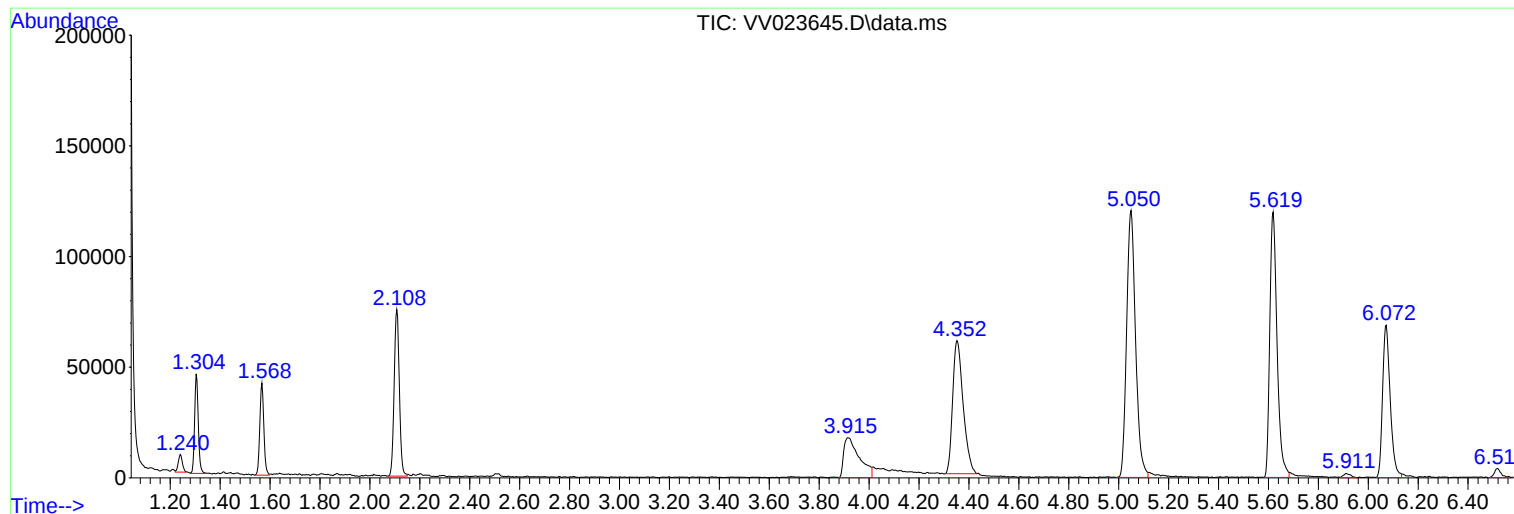

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023645.D
Acq On : 19 Nov 2021 15:52
Operator : SY/MD
Sample : M4706-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023645.D
Acq On : 19 Nov 2021 15:52
Operator : SY/MD
Sample : M4706-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
