

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023648.D
 Acq On : 19 Nov 2021 17:03
 Operator : SY/MD
 Sample : M4706-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	73	rVB	6799	7865	2.48%	0.308%
2	1.307	76	83	96	rVB	38162	40251	12.69%	1.577%
3	1.568	157	164	175	rBV	35257	40207	12.67%	1.576%
4	2.108	323	332	345	rBV	64197	91142	28.73%	3.571%
5	2.506	446	456	471	rBV	50783	85026	26.80%	3.332%
6	3.905	880	891	924	rBV2	19781	76032	23.96%	2.979%
7	4.352	1015	1030	1057	rVB4	56251	172828	54.47%	6.772%
8	5.050	1229	1247	1270	rBV3	103485	261971	82.57%	10.265%
9	5.619	1412	1424	1447	rBV	121184	248959	78.47%	9.756%
10	5.915	1506	1516	1530	rVB4	2309	4809	1.52%	0.188%
11	6.072	1550	1565	1589	rBV	61969	131531	41.46%	5.154%
12	6.519	1694	1704	1710	rBV6	2098	3461	1.09%	0.136%
13	6.989	1839	1850	1868	rBV	28915	54176	17.08%	2.123%
14	7.320	1941	1953	1972	rBV	109160	195980	61.77%	7.680%
15	7.628	2039	2049	2068	rBV3	15846	31261	9.85%	1.225%
16	8.091	2181	2193	2236	rBV	93308	245279	77.31%	9.611%
17	8.853	2416	2430	2453	rBV	191678	317268	100.00%	12.432%
18	10.217	2843	2854	2868	rBV	45727	74572	23.50%	2.922%
19	11.249	3164	3175	3195	rBV	181181	278401	87.75%	10.909%
20	11.625	3281	3292	3312	rBV	122482	190939	60.18%	7.482%




Sum of corrected areas: 2551958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023648.D
Acq On : 19 Nov 2021 17:03
Operator : SY/MD
Sample : M4706-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

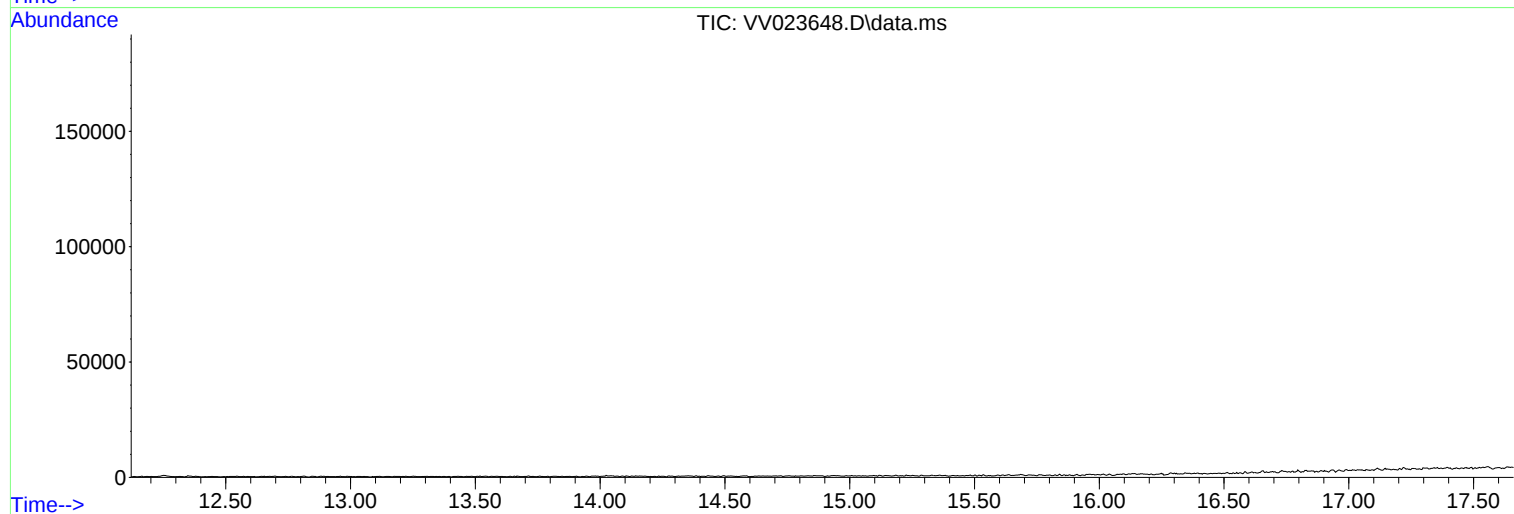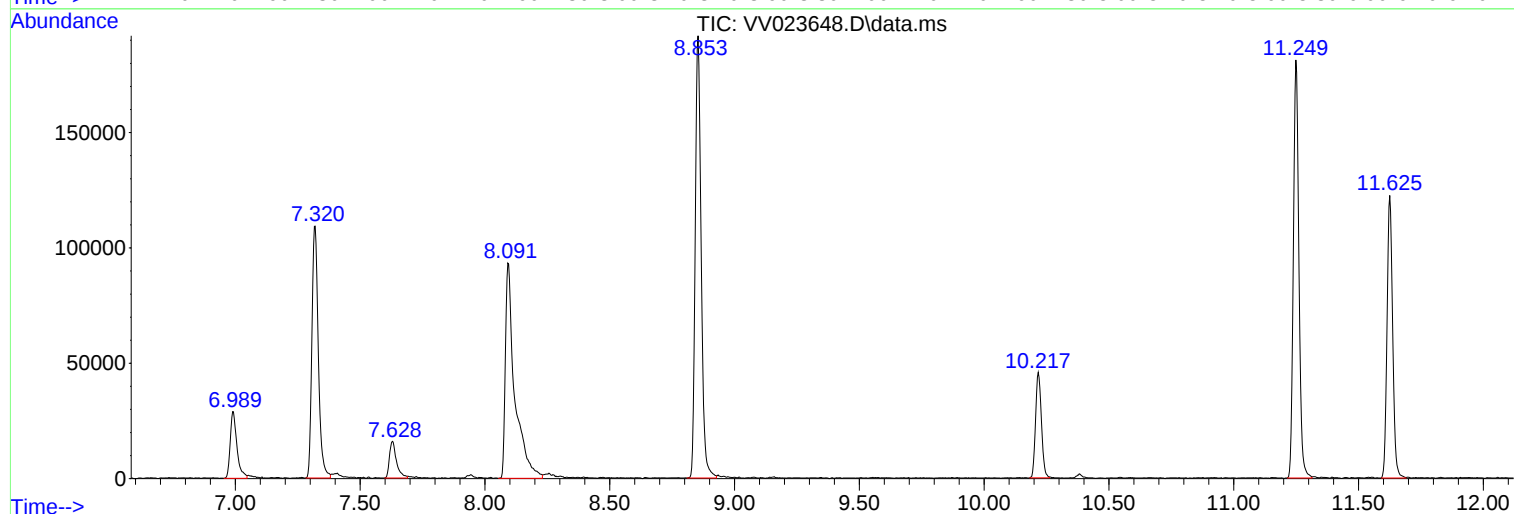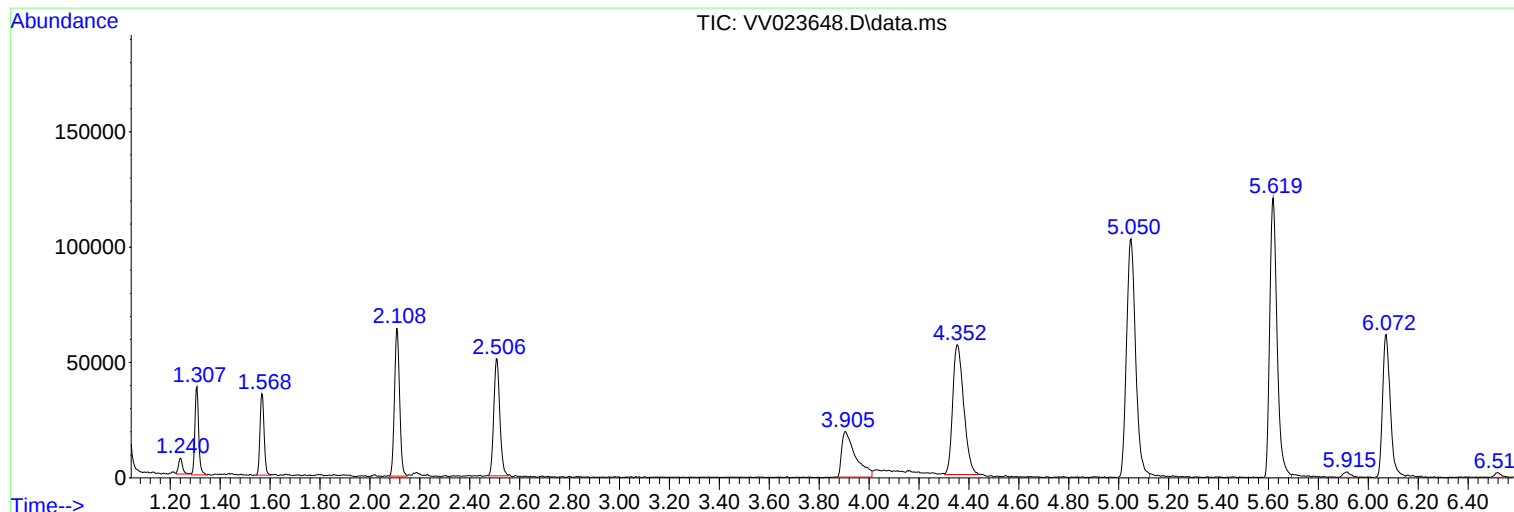

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023648.D
Acq On : 19 Nov 2021 17:03
Operator : SY/MD
Sample : M4706-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023648.D
Acq On : 19 Nov 2021 17:03
Operator : SY/MD
Sample : M4706-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
