

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
 Data File : VV023649.D
 Acq On : 19 Nov 2021 17:27
 Operator : SY/MD
 Sample : M4706-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	56	62	71	rVB	4979	5241	1.61%	0.199%
2	1.304	75	82	91	rBV	39827	39191	12.02%	1.489%
3	1.568	157	164	177	rVB	36870	41018	12.58%	1.559%
4	2.108	318	332	347	rBV	64680	96297	29.53%	3.660%
5	2.507	445	456	471	rBV	56776	94800	29.07%	3.603%
6	3.915	881	894	922	rBV2	19293	79474	24.37%	3.020%
7	4.352	1014	1030	1066	rVB3	62568	185611	56.91%	7.054%
8	5.050	1232	1247	1274	rBV2	107407	267312	81.96%	10.159%
9	5.619	1412	1424	1446	rBV2	125703	259200	79.48%	9.851%
10	5.915	1507	1516	1529	rVB4	2258	4425	1.36%	0.168%
11	6.072	1553	1565	1587	rBV	64521	134896	41.36%	5.127%
12	6.523	1696	1705	1713	rBV6	2378	3665	1.12%	0.139%
13	6.989	1841	1850	1869	rBV	28411	53761	16.48%	2.043%
14	7.317	1941	1952	1970	rBV	109314	197170	60.46%	7.493%
15	7.629	2040	2049	2061	rBV2	16587	29712	9.11%	1.129%
16	8.092	2184	2193	2229	rBV3	99107	252089	77.29%	9.580%
17	8.854	2419	2430	2453	rBV	197776	326140	100.00%	12.394%
18	10.217	2843	2854	2866	rBV	48168	77638	23.81%	2.951%
19	11.249	3165	3175	3194	rBV	184846	287600	88.18%	10.930%
20	11.625	3280	3292	3314	rBV	123821	196093	60.13%	7.452%




Sum of corrected areas: 2631333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023649.D
Acq On : 19 Nov 2021 17:27
Operator : SY/MD
Sample : M4706-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

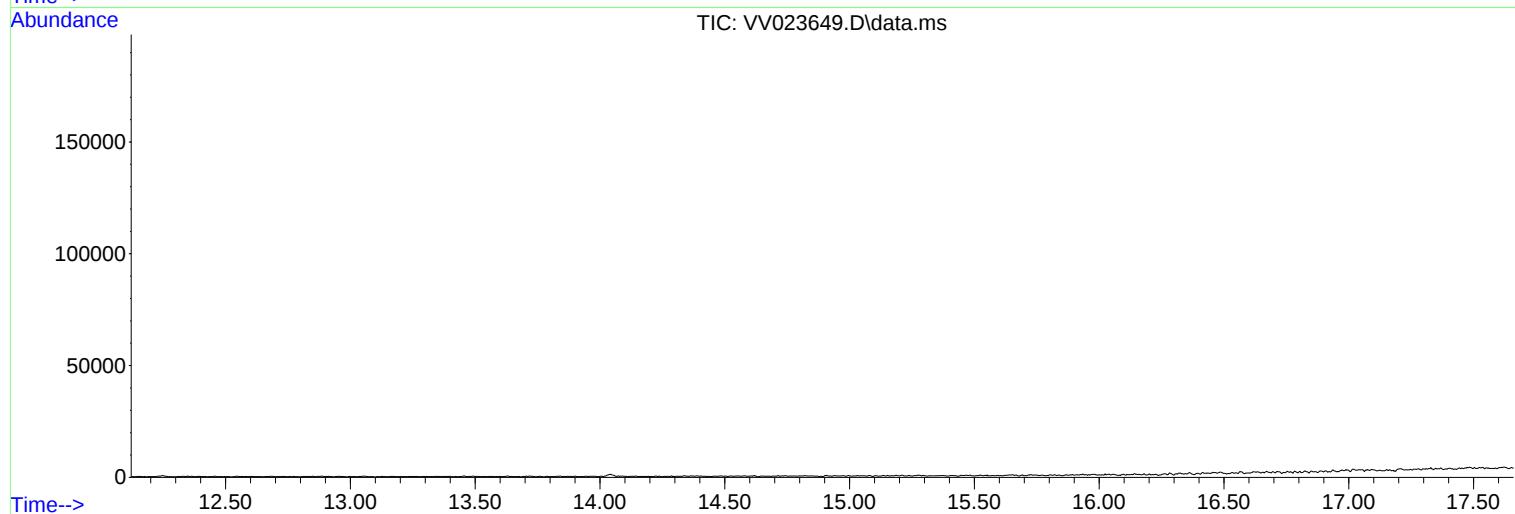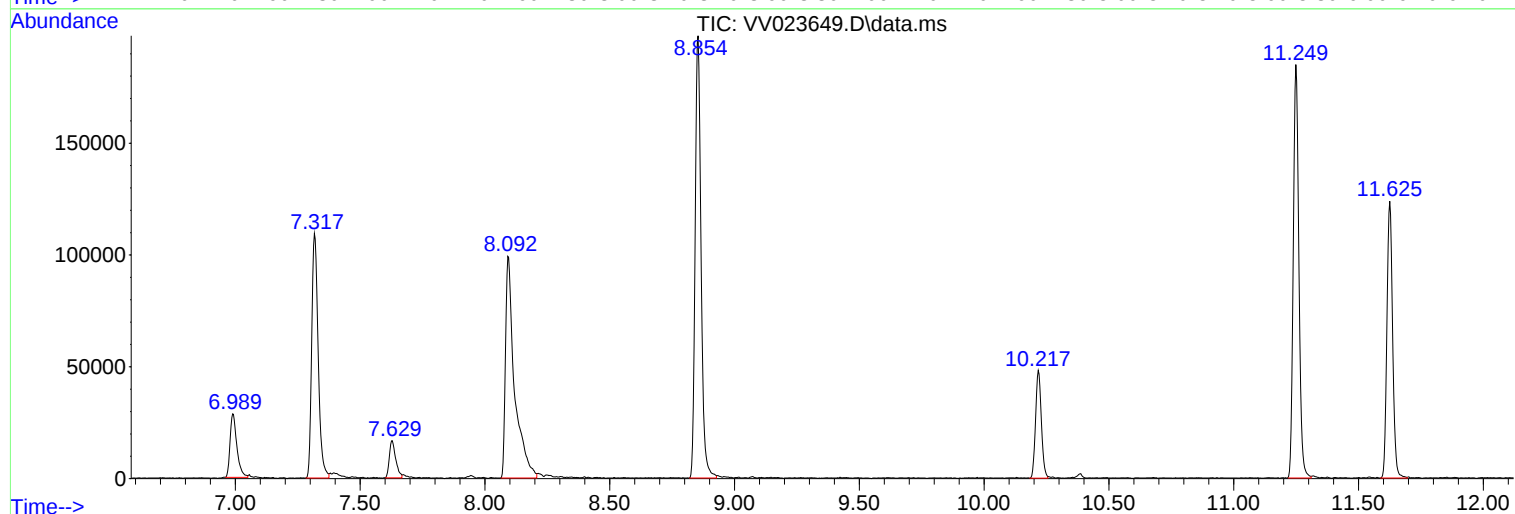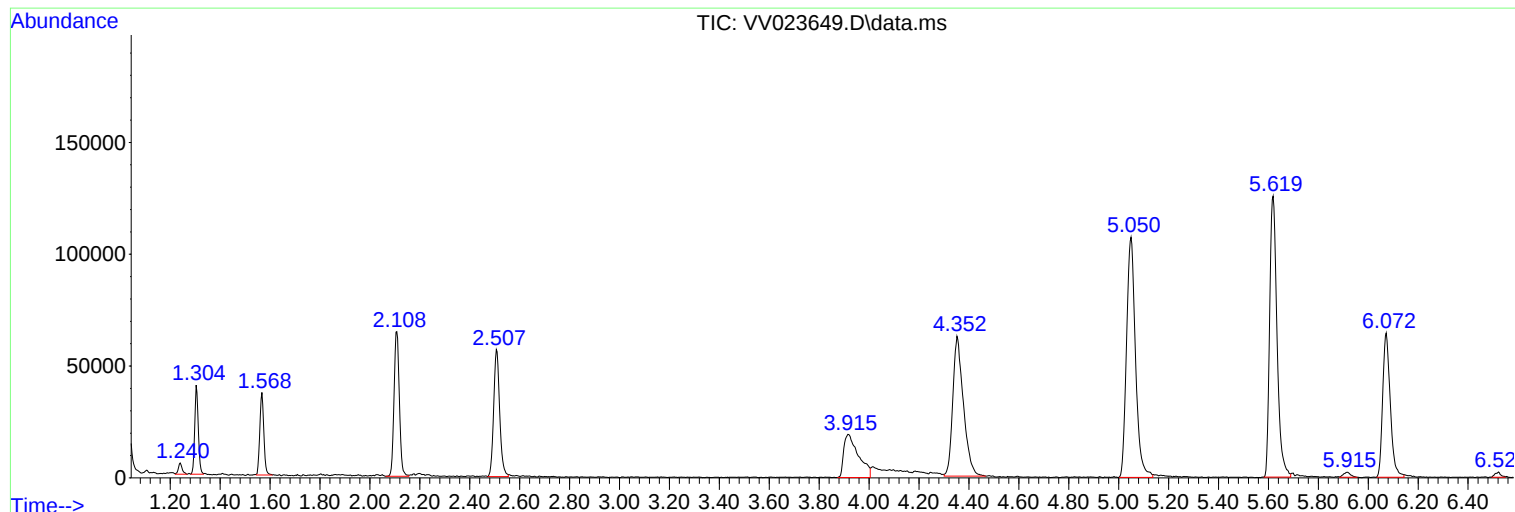

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023649.D
Acq On : 19 Nov 2021 17:27
Operator : SY/MD
Sample : M4706-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111921\
Data File : VV023649.D
Acq On : 19 Nov 2021 17:27
Operator : SY/MD
Sample : M4706-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
