

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029161.D
 Acq On : 19 Nov 2022 11:20
 Operator : SY/MD
 Sample : VV1119WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Quant Time: Nov 20 00:56:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Nov 20 00:53:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	320872	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	293321	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	134683	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	121423	6.207	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	124.200%	
7) Chloroethane-d5	1.568	69	92230	5.363	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	107.200%	
11) 1,1-Dichloroethene-d2	2.105	63	151797	4.258	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	85.200%	
20) 2-Butanone-d5	3.912	46	111511	34.053	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	68.100%	
24) Chloroform-d	4.342	84	188421	4.691	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	5.027	65	87322	4.832	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.600%	
32) Benzene-d6	5.043	84	419251	4.789	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.066	67	121527	4.971	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.400%	
41) Toluene-d8	7.310	98	371529	4.714	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
43) trans-1,3-Dichloroprop...	7.622	79	34284	4.300	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.000%	
46) 2-Hexanone-d5	8.088	63	144418	42.432	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.860%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	80274	4.736	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.615	152	125696	5.216	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	5168	0.206	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029161.D
Acq On : 19 Nov 2022 11:20
Operator : SY/MD
Sample : VV1119WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Time: Nov 20 00:56:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Nov 20 00:53:03 2022
Response via : Initial Calibration

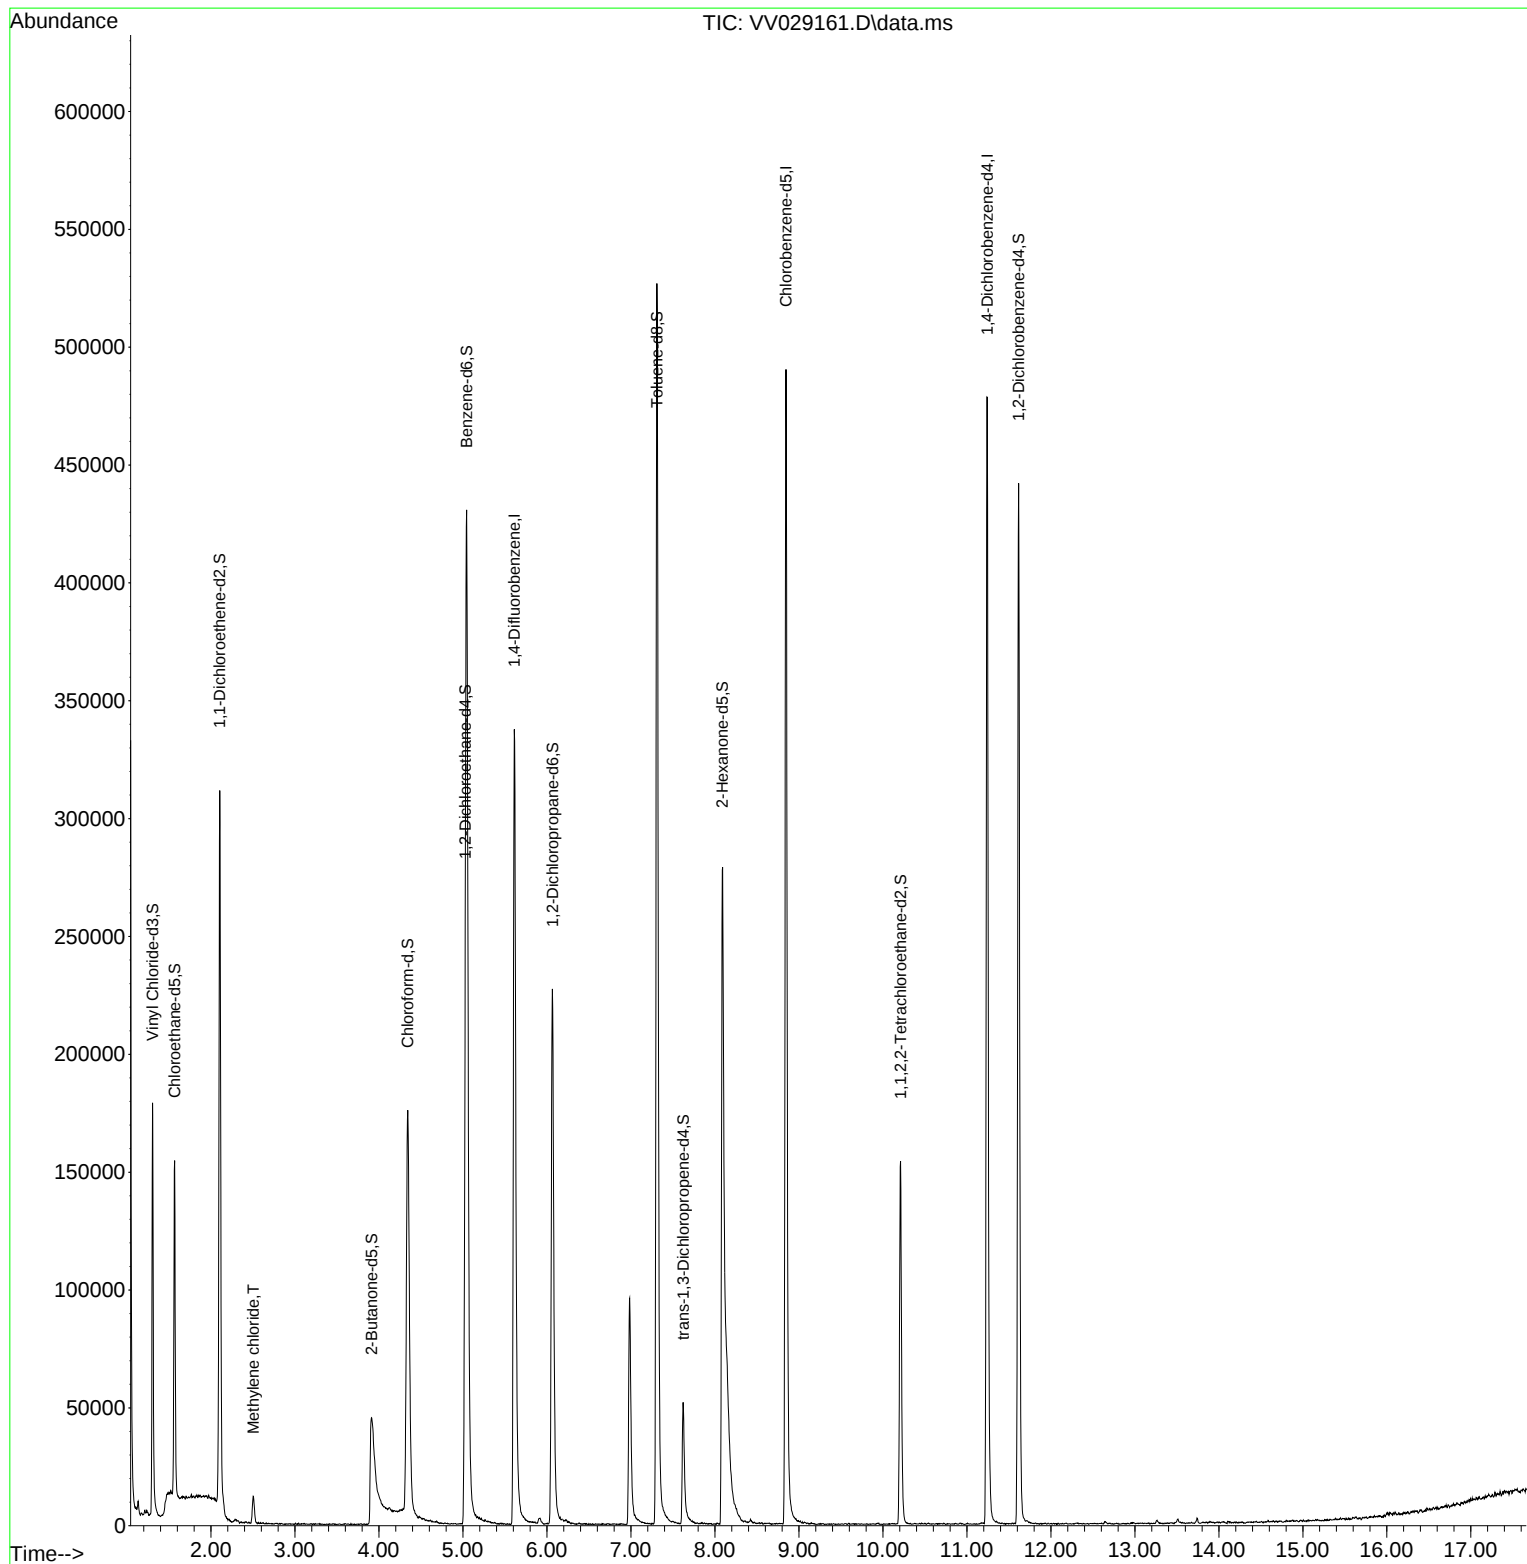

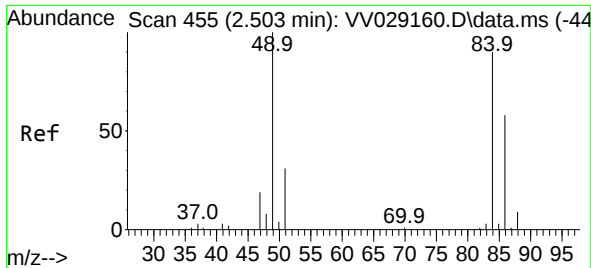

#16
Methylene chloride
Concen: 0.206 ug/L
RT: 2.503 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV029161.D
Acq: 19 Nov 2022 11:20

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Tgt Ion: 84 Resp: 5168
Ion Ratio Lower Upper
84 100
86 66.1 45.8 85.0
49 104.1 75.5 140.1

