

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW111922\  
 Data File : VW029176.D  
 Acq On : 19 Nov 2022 17:24  
 Operator : SY/MD  
 Sample : N5694-02  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BHB38

Quant Time: Nov 20 00:59:40 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR111122WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sun Nov 20 00:53:03 2022  
 Response via : Initial Calibration


| Compound                      |        | R.T.   | QIon     | Response | Conc   | Units    | Dev(Min)     |
|-------------------------------|--------|--------|----------|----------|--------|----------|--------------|
| -----                         |        |        |          |          |        |          |              |
| Internal Standards            |        |        |          |          |        |          |              |
| 1) 1,4-Difluorobenzene        |        | 5.612  | 114      | 315678   | 5.000  | ug/L     | 0.00         |
| 28) Chlorobenzene-d5          |        | 8.847  | 117      | 292388   | 5.000  | ug/L     | 0.00         |
| 58) 1,4-Dichlorobenzene-d4    |        | 11.243 | 152      | 134481   | 5.000  | ug/L     | 0.00         |
| System Monitoring Compounds   |        |        |          |          |        |          |              |
| 4) Vinyl Chloride-d3          |        | 1.307  | 65       | 106646   | 5.541  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 40 - 130 | Recovery | =      | 110.800% |              |
| 7) Chloroethane-d5            |        | 1.568  | 69       | 85137    | 5.032  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 65 - 130 | Recovery | =      | 100.600% |              |
| 11) 1,1-Dichloroethene-d2     |        | 2.108  | 63       | 134761   | 3.842  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 60 - 125 | Recovery | =      | 76.800%  |              |
| 20) 2-Butanone-d5             |        | 3.883  | 46       | 177425   | 55.074 | ug/L     | -0.01        |
| Spiked Amount                 | 50.000 | Range  | 40 - 130 | Recovery | =      | 110.140% |              |
| 24) Chloroform-d              |        | 4.342  | 84       | 182786   | 4.626  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 70 - 125 | Recovery | =      | 92.600%  |              |
| 26) 1,2-Dichloroethane-d4     |        | 5.027  | 65       | 82798    | 4.657  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 70 - 130 | Recovery | =      | 93.200%  |              |
| 32) Benzene-d6                |        | 5.047  | 84       | 388330   | 4.450  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 70 - 125 | Recovery | =      | 89.000%  |              |
| 36) 1,2-Dichloropropane-d6    |        | 6.066  | 67       | 114633   | 4.704  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 60 - 140 | Recovery | =      | 94.000%  |              |
| 41) Toluene-d8                |        | 7.310  | 98       | 337280   | 4.293  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 70 - 130 | Recovery | =      | 85.800%  |              |
| 43) trans-1,3-Dichloroprop... |        | 7.622  | 79       | 34671    | 4.362  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 55 - 130 | Recovery | =      | 87.200%  |              |
| 46) 2-Hexanone-d5             |        | 8.088  | 63       | 146513   | 43.185 | ug/L     | 0.00         |
| Spiked Amount                 | 50.000 | Range  | 45 - 130 | Recovery | =      | 86.360%  |              |
| 56) 1,1,2,2-Tetrachloroeth... |        | 10.210 | 84       | 78716    | 4.659  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 65 - 120 | Recovery | =      | 93.200%  |              |
| 66) 1,2-Dichlorobenzene-d4    |        | 11.615 | 152      | 117657   | 4.890  | ug/L     | 0.00         |
| Spiked Amount                 | 5.000  | Range  | 80 - 120 | Recovery | =      | 97.800%  |              |
| Target Compounds              |        |        |          |          |        |          |              |
| 13) Acetone                   |        | 2.175  | 43       | 10326    | 4.983  | ug/L     | Qvalue<br>85 |
| -----                         |        |        |          |          |        |          |              |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111922\  
Data File : VV029176.D  
Acq On : 19 Nov 2022 17:24  
Operator : SY/MD  
Sample : N5694-02  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BHB38

Quant Time: Nov 20 00:59:40 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR111122WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sun Nov 20 00:53:03 2022  
Response via : Initial Calibration

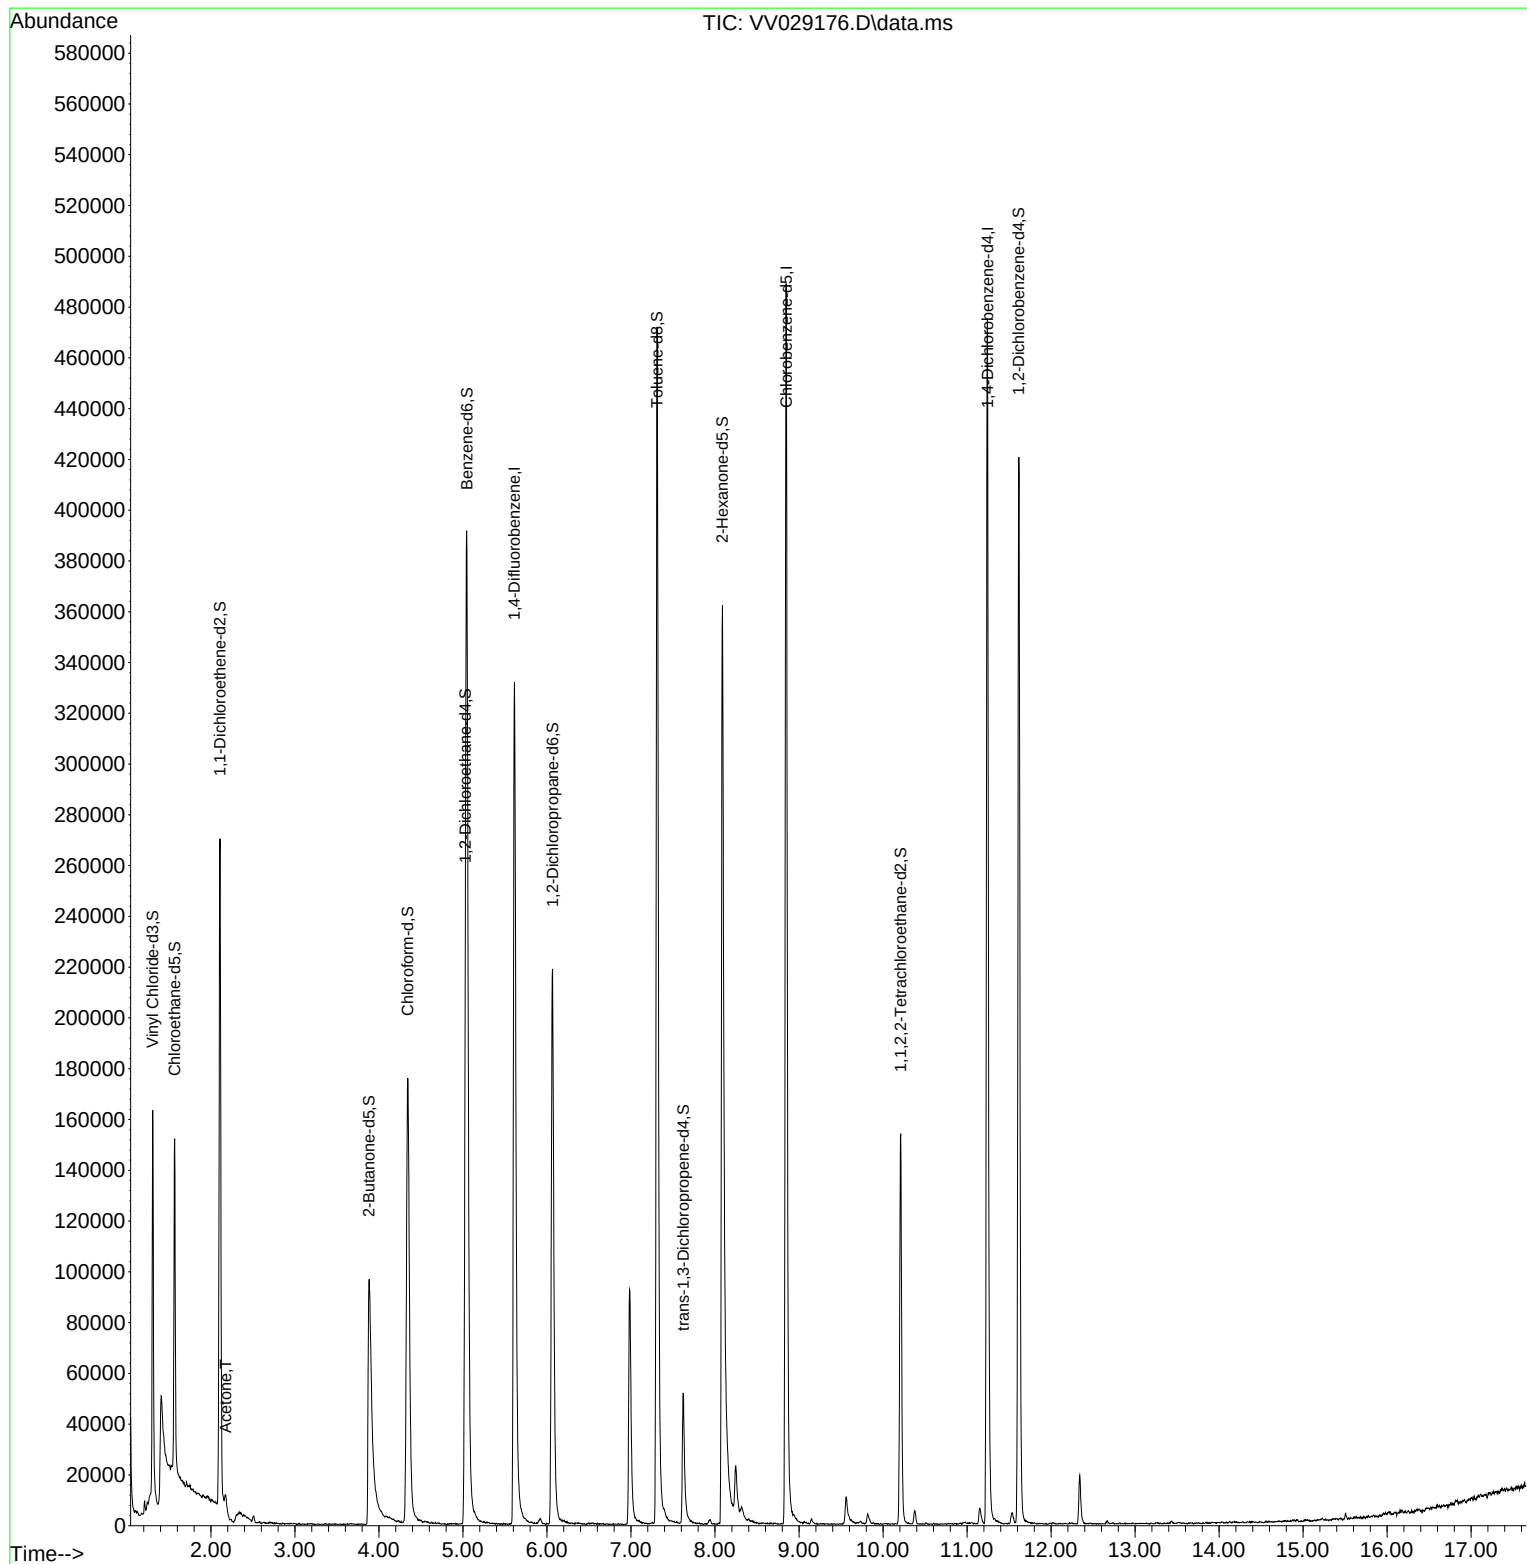

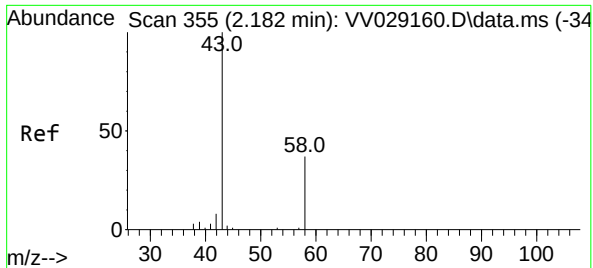

#13  
 Acetone  
 Concen: 4.983 ug/L  
 RT: 2.175 min Scan# 31  
 Delta R.T. -0.007 min  
 Lab File: VV029176.D  
 Acq: 19 Nov 2022 17:24

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BHB38

Tgt Ion: 43 Resp: 10326  
 Ion Ratio Lower Upper  
 43 100  
 58 36.1 0.0 56.6

