

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111922\
 Data File : VW029177.D
 Acq On : 19 Nov 2022 17:48
 Operator : SY/MD
 Sample : N5694-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB39

Quant Time: Nov 20 00:59:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Nov 20 00:53:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	312827	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	293269	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	135922	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	107073	5.614	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	112.200%	
7) Chloroethane-d5	1.568	69	84834	5.060	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.105	63	134004	3.856	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.200%	
20) 2-Butanone-d5	3.896	46	171568	53.741	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.480%	
24) Chloroform-d	4.343	84	181535	4.636	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.800%	
26) 1,2-Dichloroethane-d4	5.031	65	83896	4.762	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.200%	
32) Benzene-d6	5.047	84	380926	4.352	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.000%	
36) 1,2-Dichloropropane-d6	6.066	67	113624	4.648	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.000%	
41) Toluene-d8	7.310	98	334738	4.248	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	7.622	79	33767	4.236	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.088	63	151130	44.412	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.820%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	76727	4.527	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.600%	
66) 1,2-Dichlorobenzene-d4	11.616	152	117499	4.832	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	8548	4.162	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029177.D
Acq On : 19 Nov 2022 17:48
Operator : SY/MD
Sample : N5694-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB39

Quant Time: Nov 20 00:59:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Nov 20 00:53:03 2022
Response via : Initial Calibration

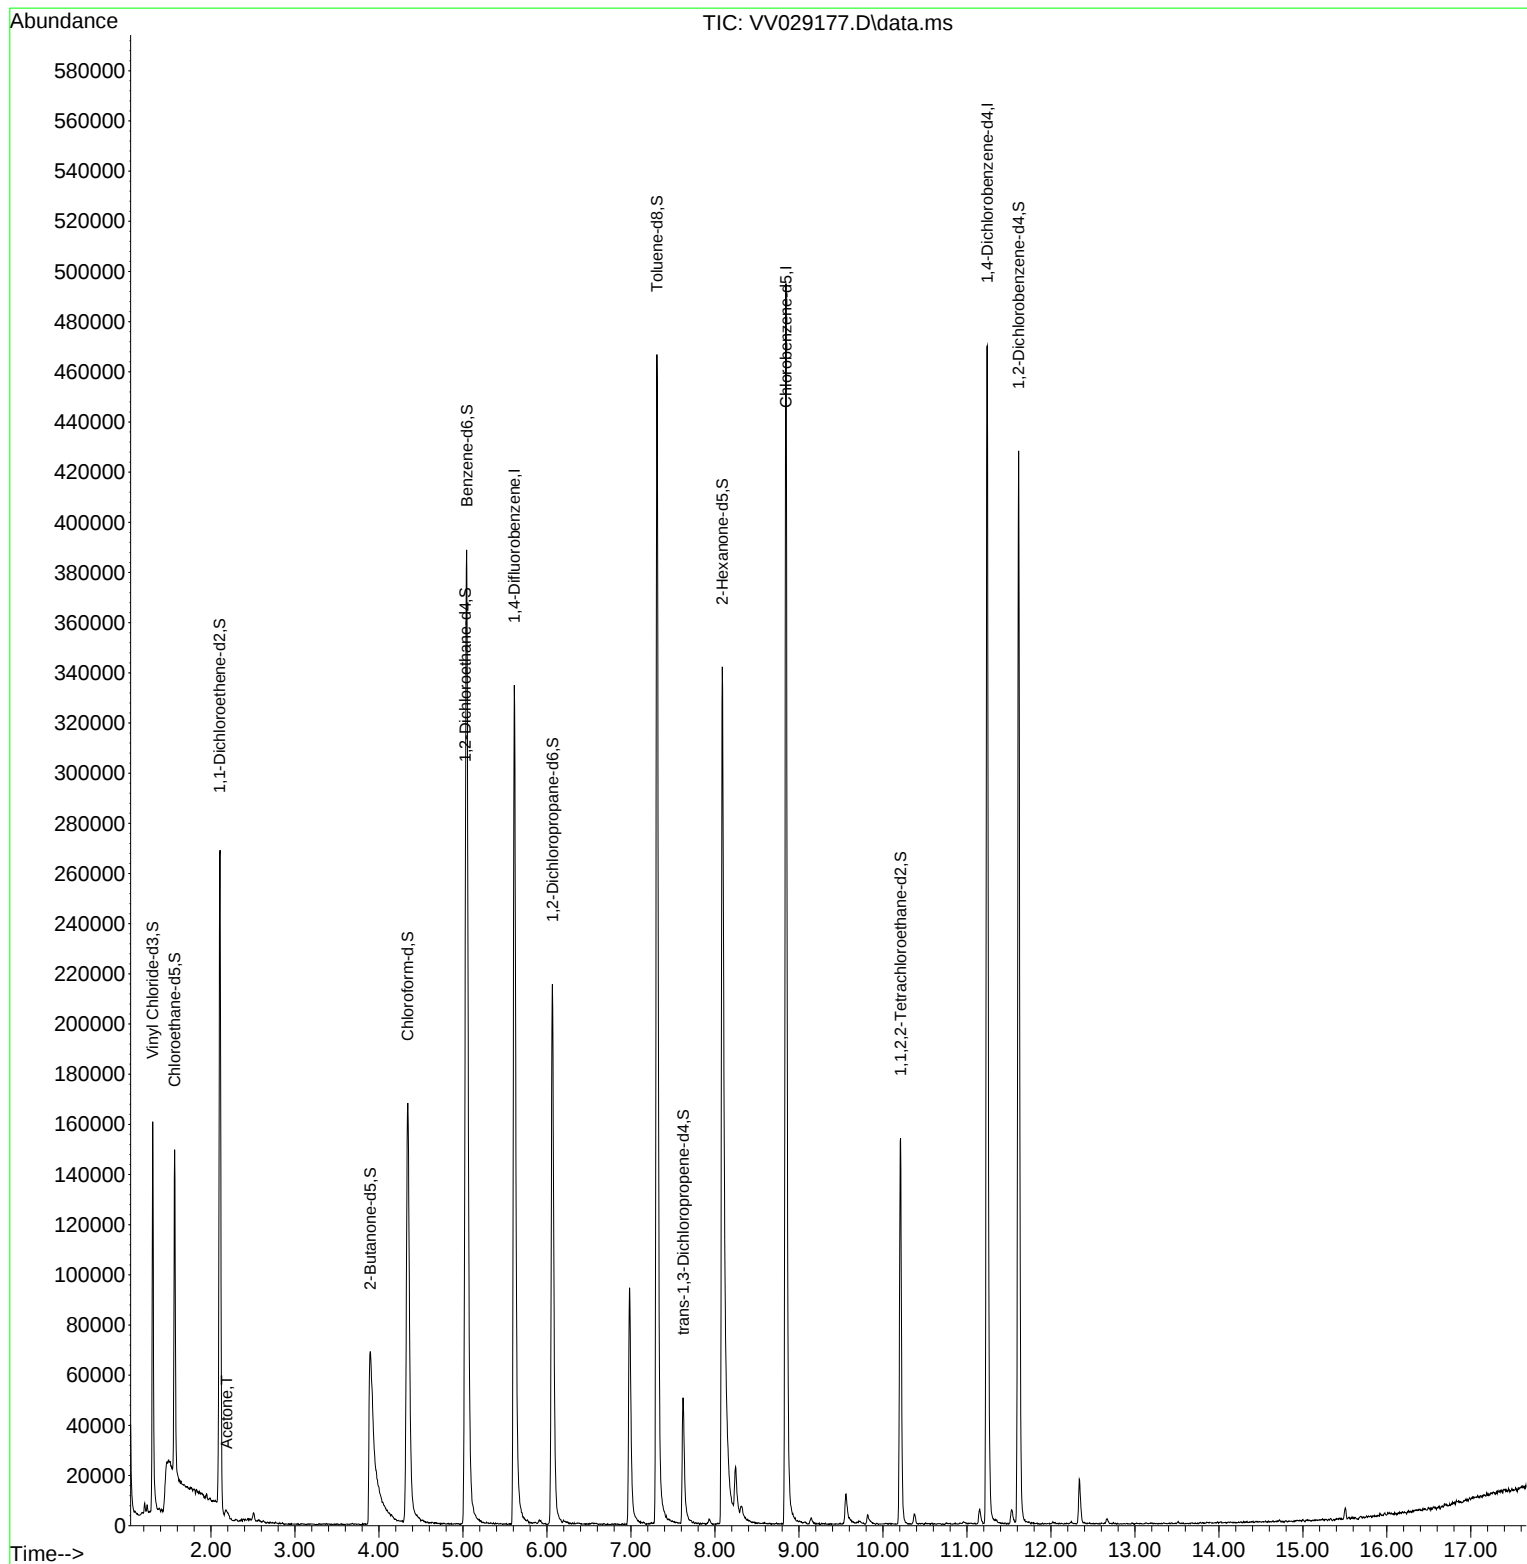

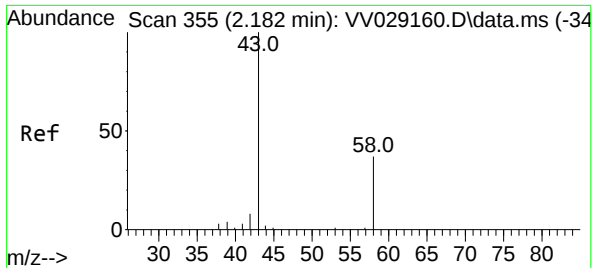

#13
 Acetone
 Concen: 4.162 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV029177.D
 Acq: 19 Nov 2022 17:48

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB39

Tgt Ion: 43 Resp: 8548
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 56.6

