

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111922\
 Data File : VW029183.D
 Acq On : 19 Nov 2022 20:14
 Operator : SY/MD
 Sample : N5694-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB45

Quant Time: Nov 20 01:01:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Nov 20 00:53:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	324666	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	298244	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	144572	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	101379	5.122	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.400%	
7) Chloroethane-d5	1.568	69	83802	4.816	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.400%	
11) 1,1-Dichloroethene-d2	2.108	63	137622	3.815	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	76.400%	
20) 2-Butanone-d5	3.883	46	183625	55.421	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	110.840%	
24) Chloroform-d	4.343	84	179576	4.419	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.400%	
26) 1,2-Dichloroethane-d4	5.027	65	80393	4.397	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.000%	
32) Benzene-d6	5.047	84	387560	4.354	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.000%	
36) 1,2-Dichloropropane-d6	6.066	67	112649	4.532	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.600%	
41) Toluene-d8	7.310	98	338687	4.226	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.600%	
43) trans-1,3-Dichloroprop...	7.622	79	32127	3.963	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.200%	
46) 2-Hexanone-d5	8.085	63	144016	41.615	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.240%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	73377	4.258	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	85.200%	
66) 1,2-Dichlorobenzene-d4	11.616	152	126241	4.881	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.600%	
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.118	96	14624	0.744	ug/L	# 1
13) Acetone	2.172	43	9923	4.656	ug/L	86
17) Methyl tert-butyl Ether	2.764	73	17807	0.423	ug/L	96
19) 1,1-Dichloroethane	3.188	63	82492	2.214	ug/L	98
22) cis-1,2-Dichloroethene	3.905	96	183561	7.921	ug/L	98
29) 1,1,1-Trichloroethane	4.609	97	5986	0.171	ug/L	99
34) Trichloroethene	5.918	95	24420	1.047	ug/L	98
42) Toluene	7.391	91	23066	0.234	ug/L	100
52) Ethylbenzene	9.014	91	12837	0.125	ug/L	99
53) m,p-Xylene	9.137	106	16623	0.408	ug/L	93
54) o-Xylene	9.542	106	8307	0.214	ug/L	98
62) 1,3,5-Trimethylbenzene	10.535	105	6687	0.084	ug/L	98
63) 1,2,4-Trimethylbenzene	10.911	105	22297	0.280	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029183.D
Acq On : 19 Nov 2022 20:14
Operator : SY/MD
Sample : N5694-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB45

Quant Time: Nov 20 01:01:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Nov 20 00:53:03 2022
Response via : Initial Calibration

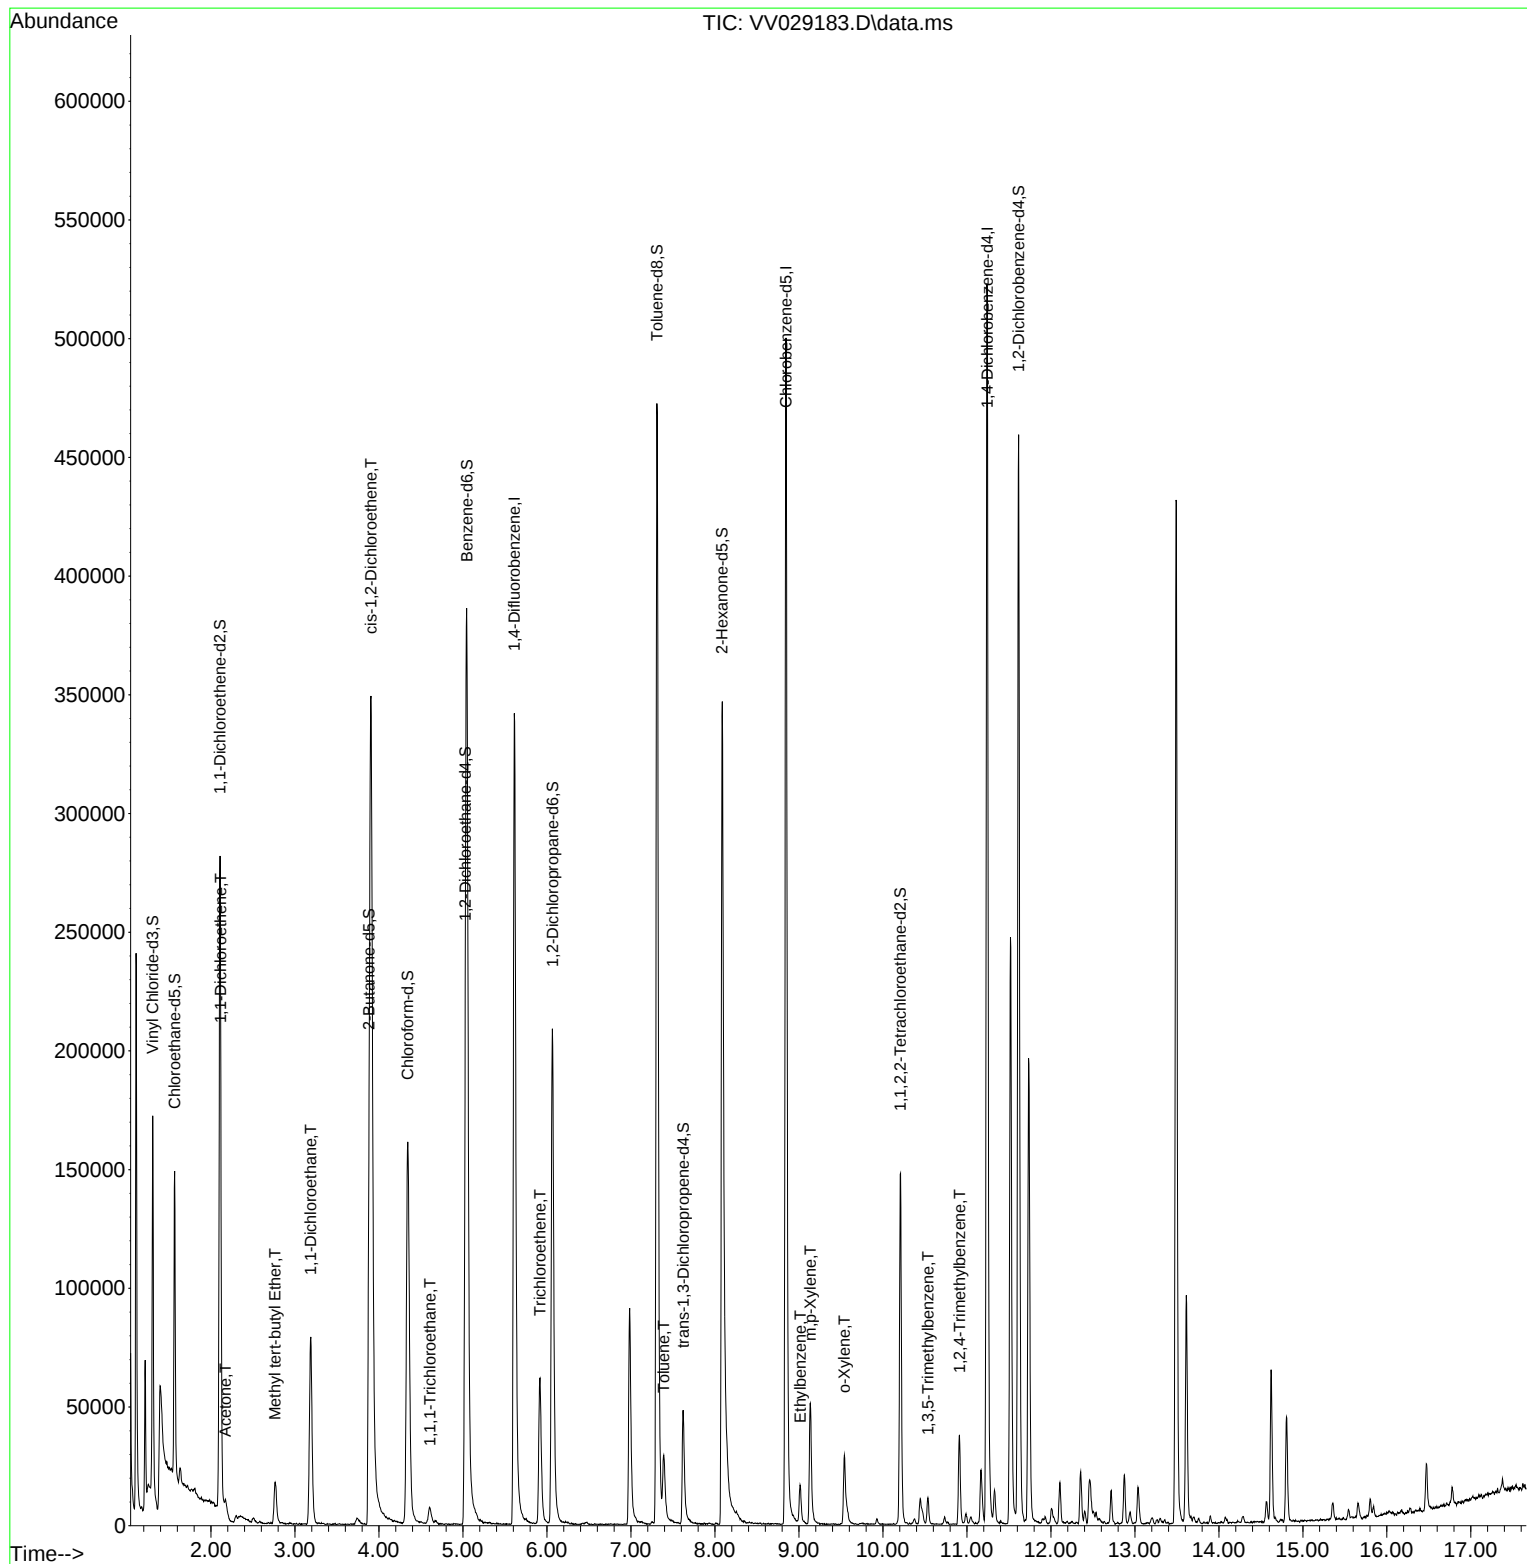

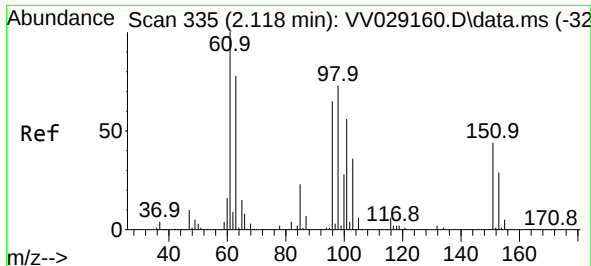

#12

1,1-Dichloroethene

Concen: 0.744 ug/L

RT: 2.118 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV029183.D

Acq: 19 Nov 2022 20:14

Instrument :

MSVOA_V

ClientSampleId :

BHB45





Tgt Ion: 96 Resp: 14624

Ion Ratio Lower Upper

96 100

61 195.6 104.2 193.4#

63 551.8 75.9 140.9#

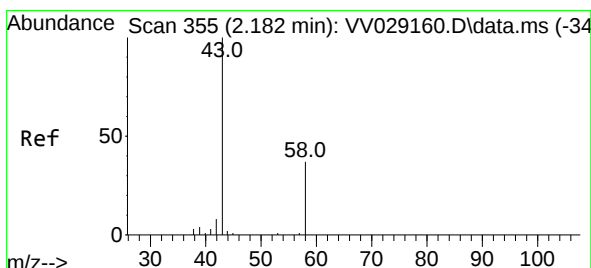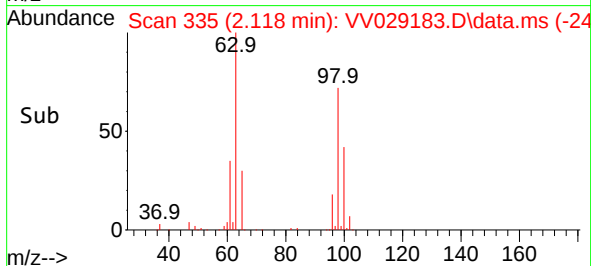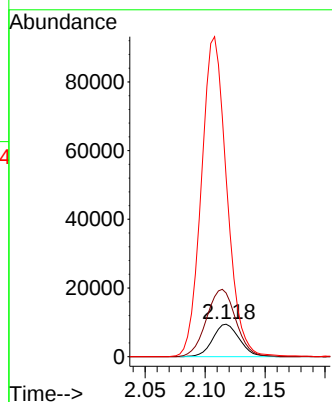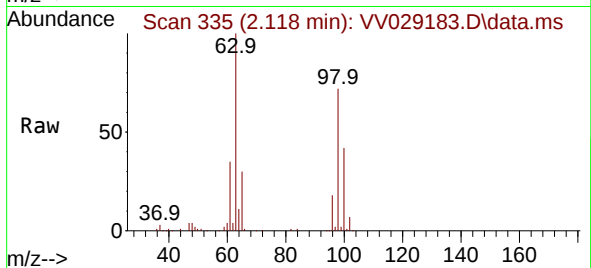

#13

Acetone

Concen: 4.656 ug/L

RT: 2.172 min Scan# 352

Delta R.T. -0.010 min

Lab File: VV029183.D




Acq: 19 Nov 2022 20:14


Tgt Ion: 43 Resp: 9923

Ion Ratio Lower Upper

43 100

58 35.5 0.0 56.6

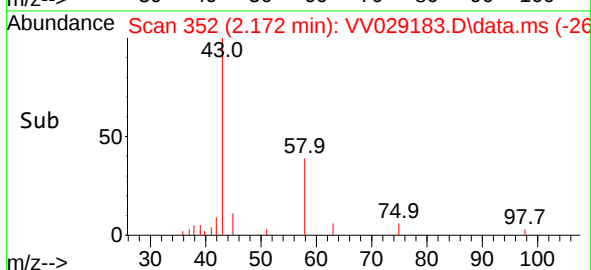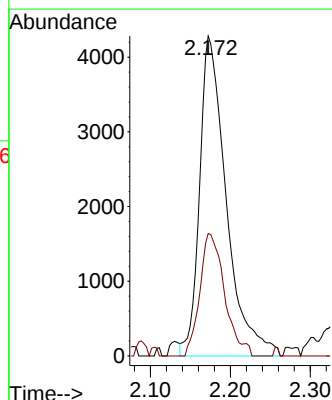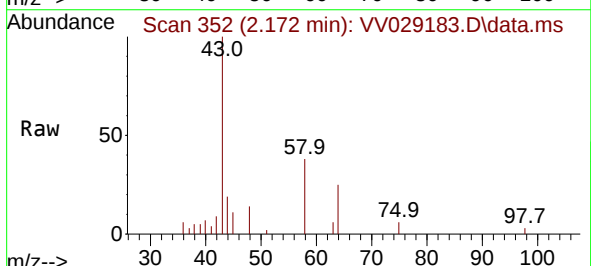

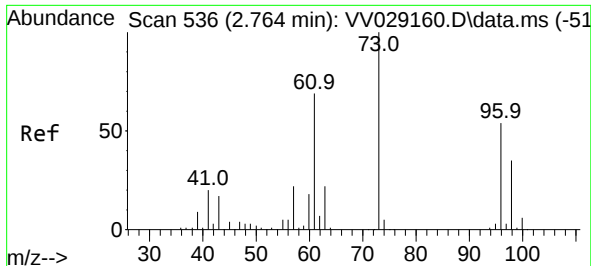

#17

Methyl tert-butyl Ether

Concen: 0.423 ug/L

RT: 2.764 min Scan# 51

Delta R.T. -0.000 min

Lab File: VV029183.D

Acq: 19 Nov 2022 20:14

Instrument :





MSVOA_V

ClientSampleId :

BHB45

Tgt Ion: 73 Resp: 17807

Ion	Ratio	Lower	Upper
73	100		
43	17.1	13.0	19.4
57	23.1	16.6	24.8

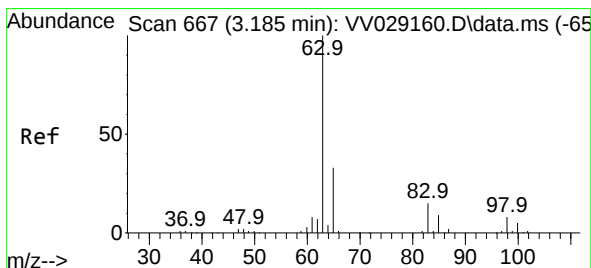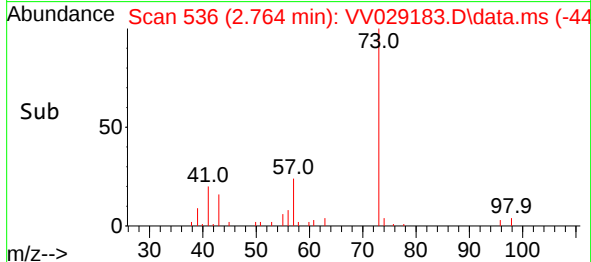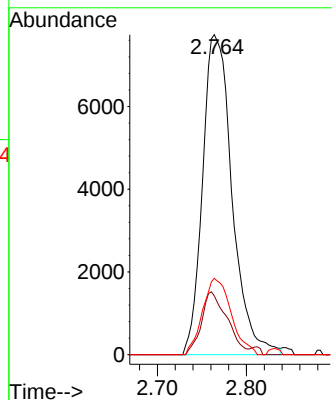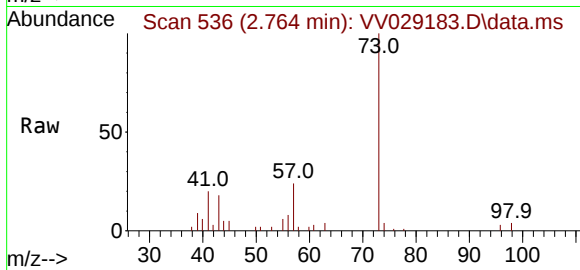

#19

1,1-Dichloroethane

Concen: 2.214 ug/L

RT: 3.188 min Scan# 668




Delta R.T. 0.003 min


Lab File: VV029183.D

Acq: 19 Nov 2022 20:14

Tgt Ion: 63 Resp: 82492

Ion	Ratio	Lower	Upper
63	100		
65	31.7	23.0	42.6
83	14.0	9.4	17.6

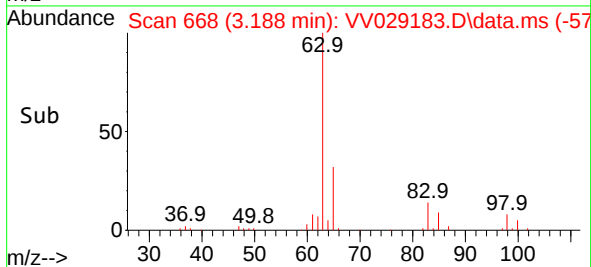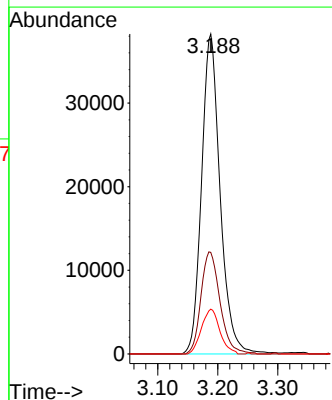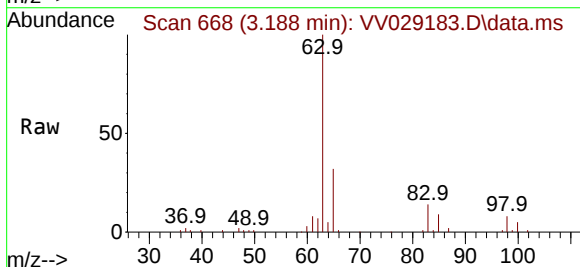

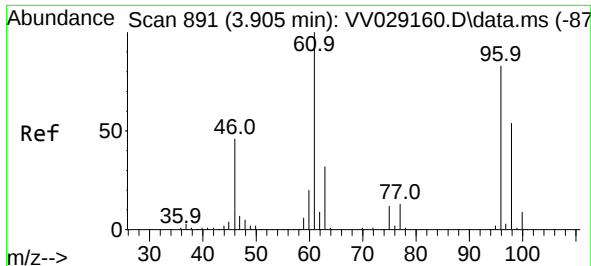

#22

cis-1,2-Dichloroethene

Concen: 7.921 ug/L

RT: 3.905 min Scan# 891

Delta R.T. -0.000 min

Lab File: VV029183.D

Acq: 19 Nov 2022 20:14

Instrument :

MSVOA_V

ClientSampleId :

BHB45





Tgt Ion: 96 Resp: 183561

Ion Ratio Lower Upper

96 100

61 120.3 82.3 152.9

68 0.0 0.0 0.0

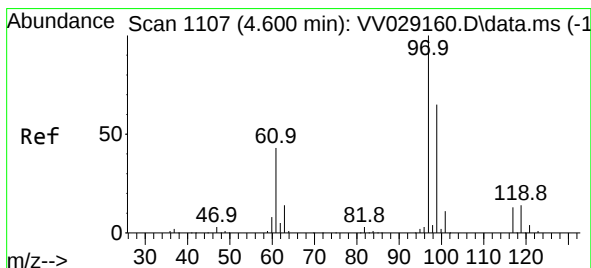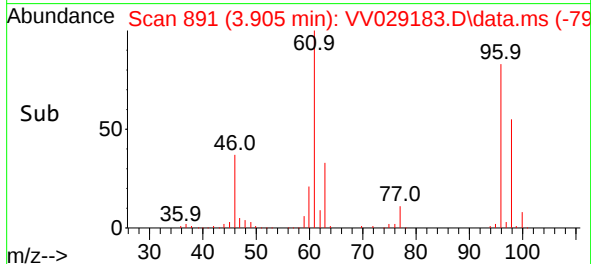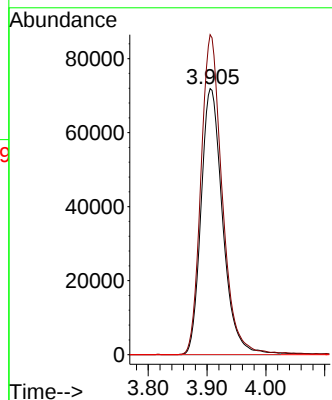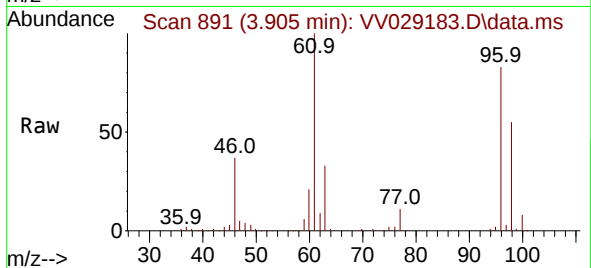

#29

1,1,1-Trichloroethane

Concen: 0.171 ug/L

RT: 4.609 min Scan# 1110

Delta R.T. 0.010 min

Lab File: VV029183.D

Acq: 19 Nov 2022 20:14




Tgt Ion: 97 Resp: 5986


Ion Ratio Lower Upper

97 100

99 65.1 52.7 79.1

61 43.4 33.8 50.6


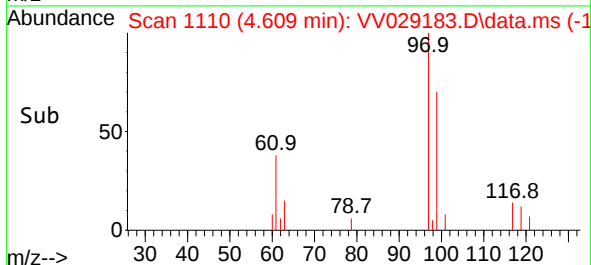
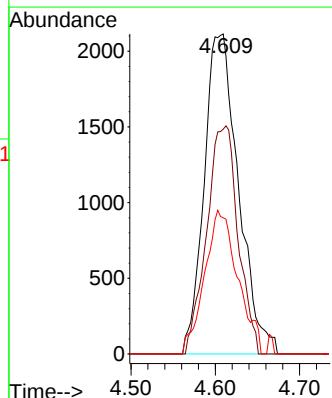
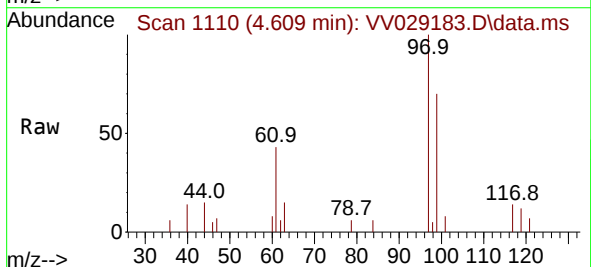


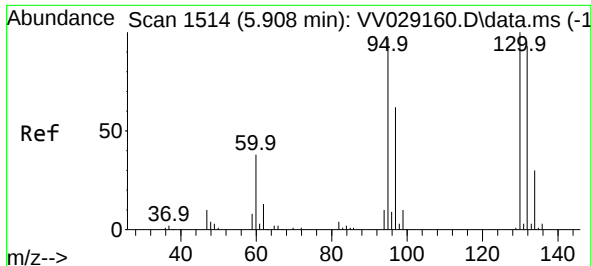

#34
 Trichloroethene
 Concen: 1.047 ug/L
 RT: 5.918 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV029183.D
 Acq: 19 Nov 2022 20:14




Instrument :
 MSVOA_V
 ClientSampleId :
 BHB45


Tgt Ion: 95 Resp: 24420
 Ion Ratio Lower Upper
 95 100
 97 62.1 45.6 84.8
 132 100.9 69.1 128.3
 130 108.3 74.9 139.1

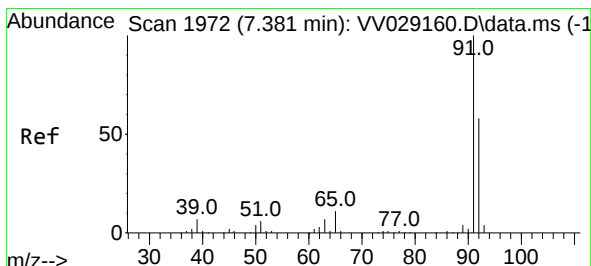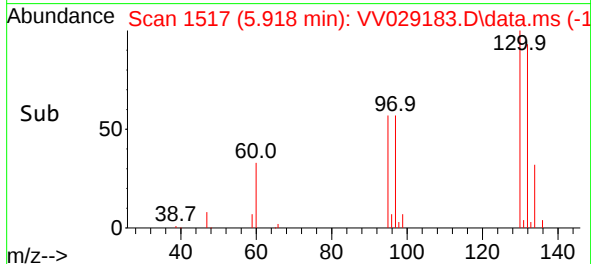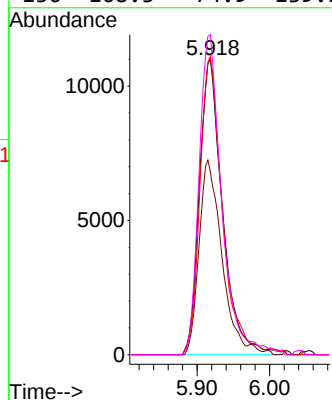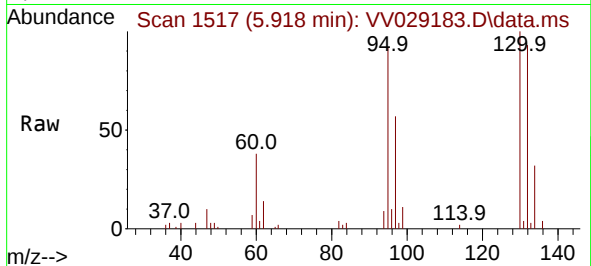

#42
 Toluene
 Concen: 0.234 ug/L
 RT: 7.391 min Scan# 1975
 Delta R.T. 0.010 min
 Lab File: VV029183.D
 Acq: 19 Nov 2022 20:14

Tgt Ion: 91 Resp: 23066
 Ion Ratio Lower Upper
 91 100
 92 58.5 40.7 75.5


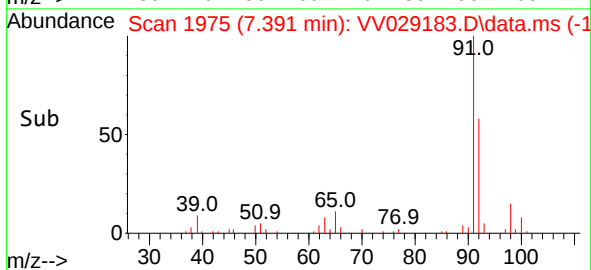
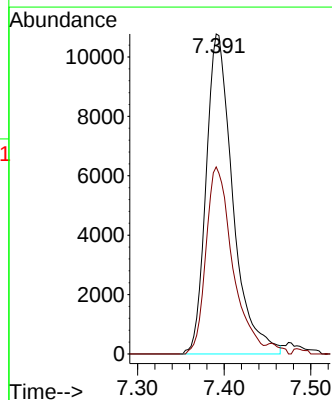
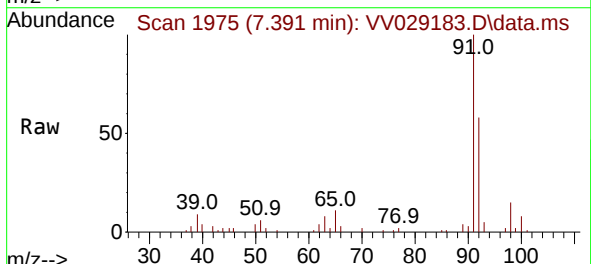


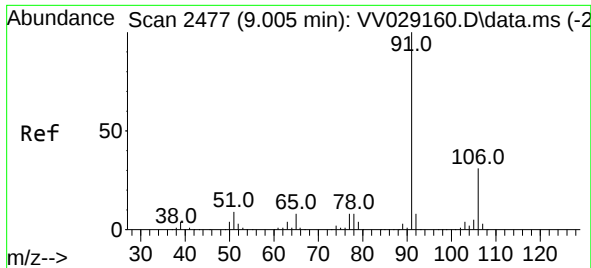

#52
Ethylbenzene
Concen: 0.125 ug/L
RT: 9.014 min Scan# 2477
Delta R.T. 0.010 min
Lab File: VV029183.D
Acq: 19 Nov 2022 20:14




Instrument :
MSVOA_V
ClientSampleId :
BHB45


Tgt Ion: 91 Resp: 12837
Ion Ratio Lower Upper
91 100
106 31.7 21.6 40.2

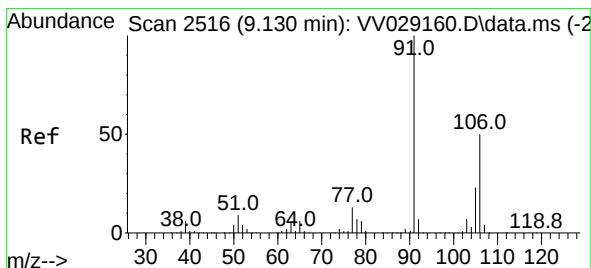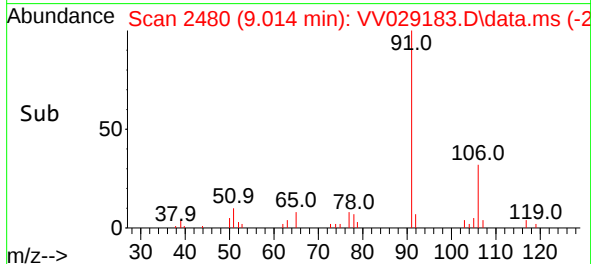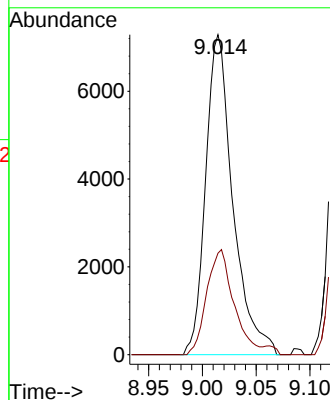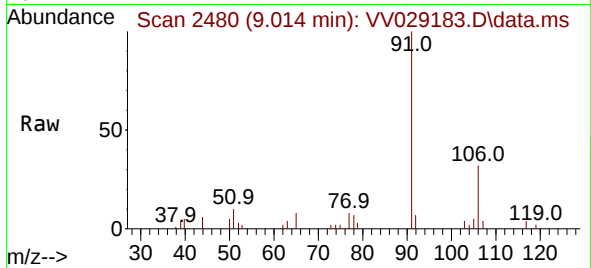

#53
m,p-Xylene
Concen: 0.408 ug/L
RT: 9.137 min Scan# 2518
Delta R.T. 0.006 min
Lab File: VV029183.D
Acq: 19 Nov 2022 20:14

Tgt Ion: 106 Resp: 16623
Ion Ratio Lower Upper
106 100
91 209.2 139.1 258.3


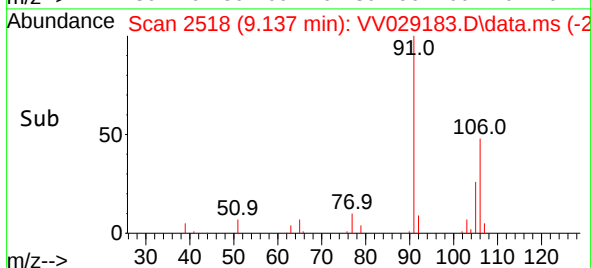
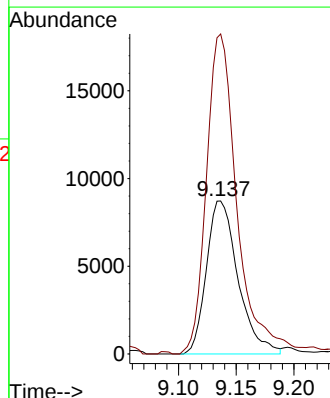
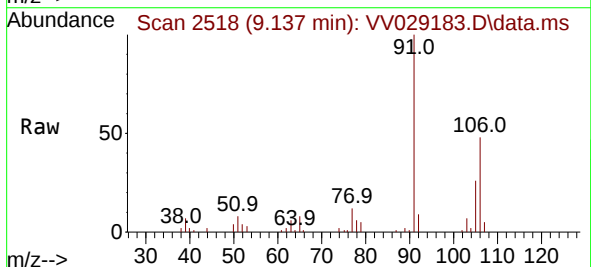


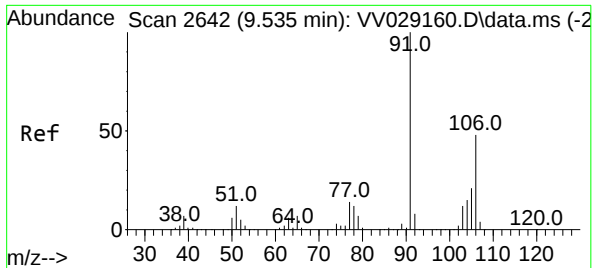

#54
o-Xylene
Concen: 0.214 ug/L
RT: 9.542 min Scan# 2106
Delta R.T. 0.006 min
Lab File: VV029183.D
Acq: 19 Nov 2022 20:14




Instrument :
MSVOA_V
ClientSampleId :
BHB45


Tgt Ion:106 Resp: 8307
Ion Ratio Lower Upper
106 100
91 211.6 145.7 270.7

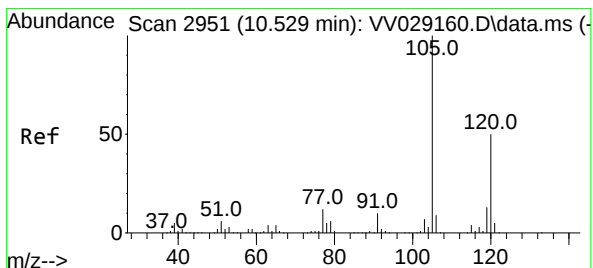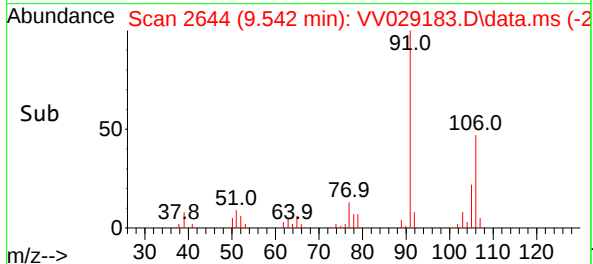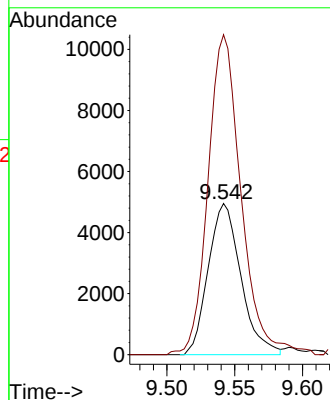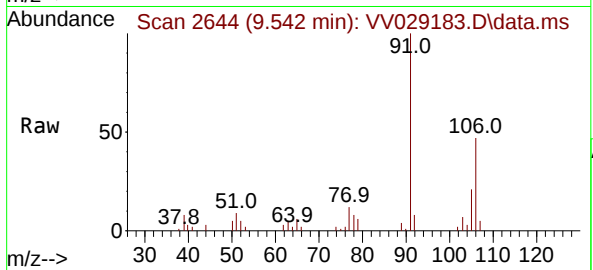

#62
1,3,5-Trimethylbenzene
Concen: 0.084 ug/L
RT: 10.535 min Scan# 2953
Delta R.T. 0.006 min
Lab File: VV029183.D
Acq: 19 Nov 2022 20:14

Tgt Ion:105 Resp: 6687
Ion Ratio Lower Upper
105 100
120 51.5 39.9 59.9

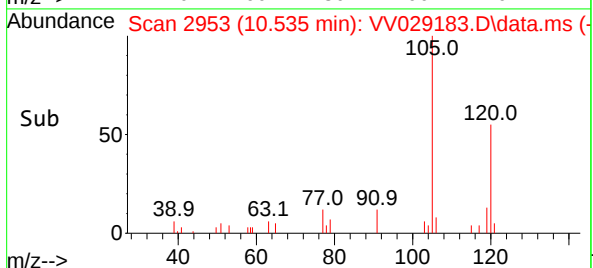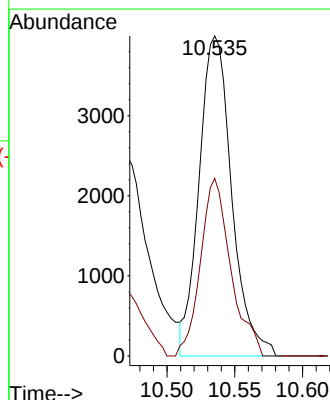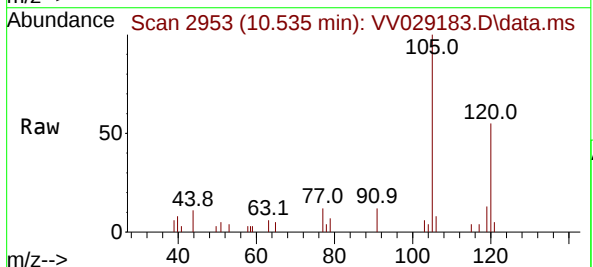

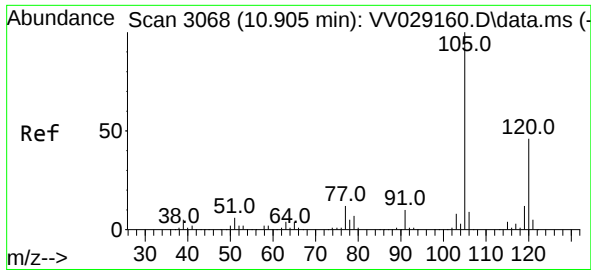

#63

1,2,4-Trimethylbenzene

Concen: 0.280 ug/L

RT: 10.911 min Scan# 30

Delta R.T. 0.006 min

Lab File: VV029183.D

Acq: 19 Nov 2022 20:14

Instrument :

MSVOA_V

ClientSampleId :

BHB45

Tgt Ion:105 Resp: 22297

Ion Ratio Lower Upper

105 100

120 44.6 37.8 56.8

