

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029170.D
 Acq On : 19 Nov 2022 14:57
 Operator : SY/MD
 Sample : N5687-19DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCE4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rBV	152924	161340	16.44%	1.737%
2	1.568	156	164	177	rBV	130942	149912	15.28%	1.614%
3	2.108	321	332	348	rVB	266169	400977	40.86%	4.316%
4	2.506	445	456	471	rBV	30754	53621	5.46%	0.577%
5	3.908	877	892	933	rBV4	137366	451368	46.00%	4.859%
6	4.342	1012	1027	1057	rVB	163770	415184	42.31%	4.469%
7	4.603	1095	1108	1124	rVB3	19085	47846	4.88%	0.515%
8	5.043	1229	1245	1279	rBV2	386510	981277	100.00%	10.563%
9	5.612	1411	1422	1452	rBV	342387	715671	72.93%	7.704%
10	5.908	1501	1514	1550	rBV	489833	980920	99.96%	10.559%
11	6.066	1550	1563	1596	rVB	211010	448329	45.69%	4.826%
12	6.985	1838	1849	1872	rBV	93744	181639	18.51%	1.955%
13	7.310	1939	1950	2000	rBV	469311	855927	87.23%	9.214%
14	7.622	2037	2047	2070	rBV	50358	98921	10.08%	1.065%
15	8.091	2182	2193	2248	rBV3	248130	803097	81.84%	8.645%
16	8.847	2416	2428	2457	rBV	491067	838236	85.42%	9.024%
17	10.210	2840	2852	2878	rBV	144374	247808	25.25%	2.668%
18	11.239	3162	3172	3198	rBV	472450	776074	79.09%	8.354%
19	11.615	3277	3289	3311	rBV	419997	681314	69.43%	7.334%




Sum of corrected areas: 9289461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029170.D
Acq On : 19 Nov 2022 14:57
Operator : SY/MD
Sample : N5687-19DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

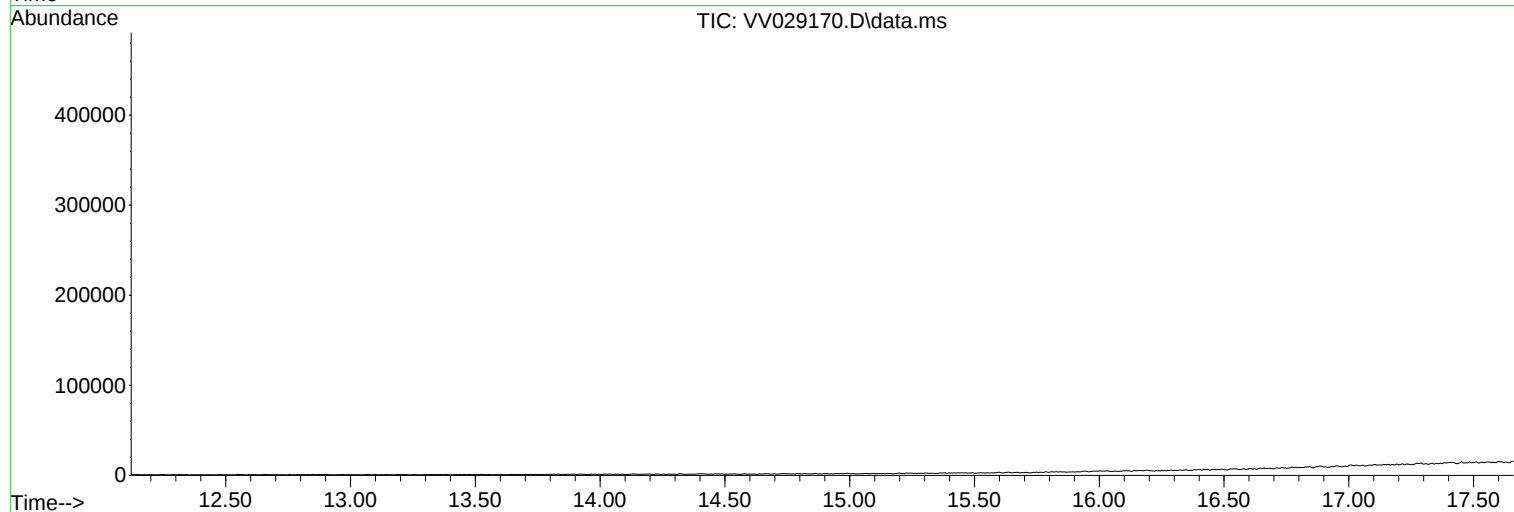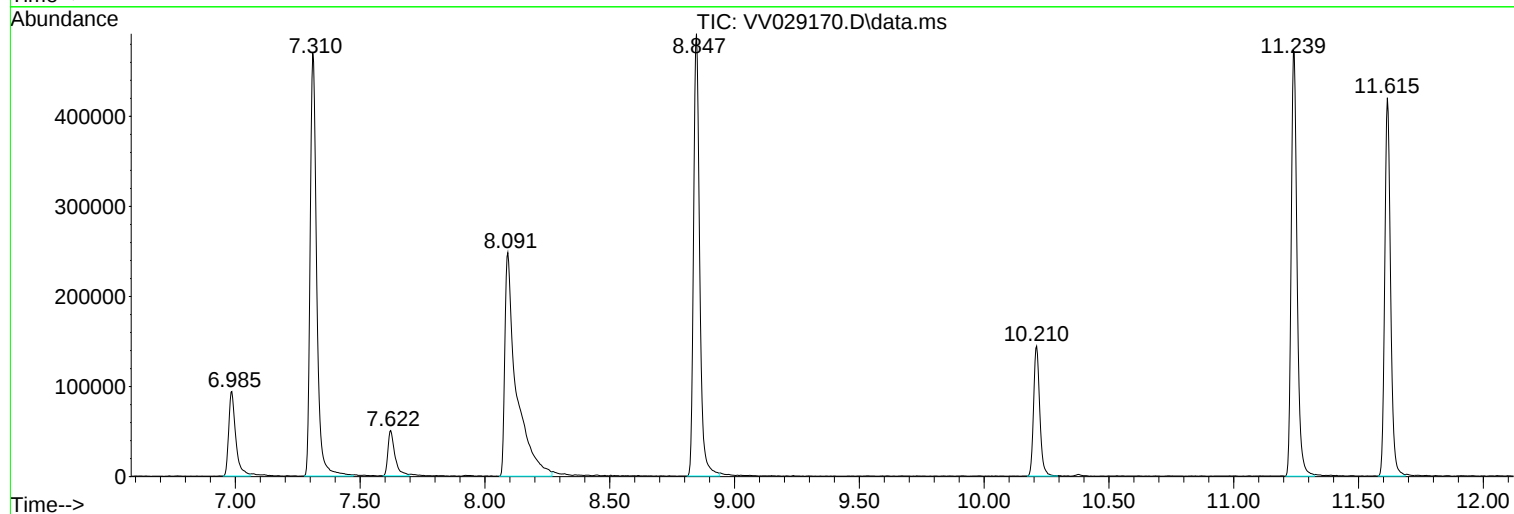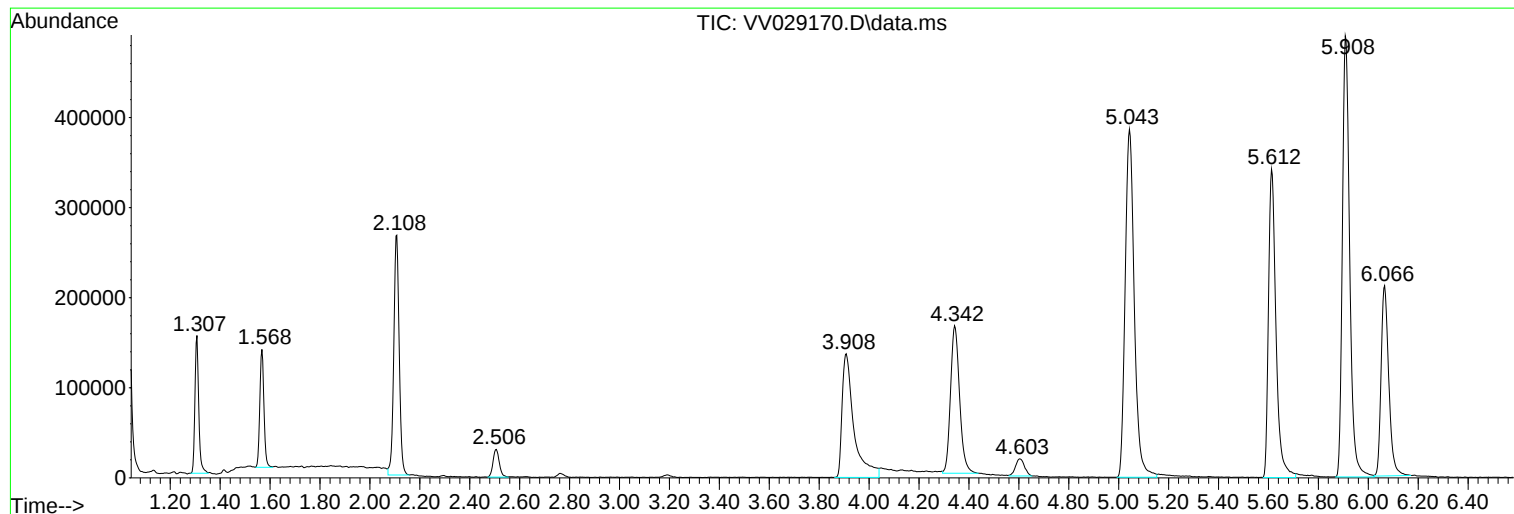

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029170.D
Acq On : 19 Nov 2022 14:57
Operator : SY/MD
Sample : N5687-19DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029170.D
Acq On : 19 Nov 2022 14:57
Operator : SY/MD
Sample : N5687-19DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc