

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029189.D
 Acq On : 19 Nov 2022 22:53
 Operator : SY/MD
 Sample : N5648-03DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46D4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	104	rBV2	191961	218854	19.31%	2.168%
2	1.568	156	164	177	rVB	124387	145464	12.84%	1.441%
3	2.105	321	331	352	rVB	256282	388540	34.29%	3.849%
4	2.503	445	455	467	rBV	16424	29104	2.57%	0.288%
5	2.764	522	536	558	rBV2	70383	150025	13.24%	1.486%
6	3.905	874	891	928	rBV2	415064	1133237	100.00%	11.227%
7	4.342	1012	1027	1066	rVB	161467	421024	37.15%	4.171%
8	5.043	1226	1245	1281	rBV2	379086	962210	84.91%	9.533%
9	5.612	1410	1422	1459	rBV	335852	701998	61.95%	6.955%
10	5.908	1502	1514	1547	rBV	568327	1124915	99.27%	11.145%
11	6.066	1550	1563	1591	rVV	206427	434152	38.31%	4.301%
12	6.982	1837	1848	1869	rBV	89431	174900	15.43%	1.733%
13	7.310	1939	1950	1973	rBV	454931	814759	71.90%	8.072%
14	7.622	2036	2047	2075	rBV2	45729	92652	8.18%	0.918%
15	8.088	2182	2192	2242	rBV	279918	807990	71.30%	8.005%
16	8.847	2416	2428	2461	rBV	472766	809060	71.39%	8.016%
17	10.210	2840	2852	2877	rBV	144650	247111	21.81%	2.448%
18	11.239	3162	3172	3191	rBV	471687	759999	67.06%	7.529%
19	11.615	3274	3289	3309	rBV	422473	677660	59.80%	6.714%




Sum of corrected areas: 10093654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029189.D
Acq On : 19 Nov 2022 22:53
Operator : SY/MD
Sample : N5648-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

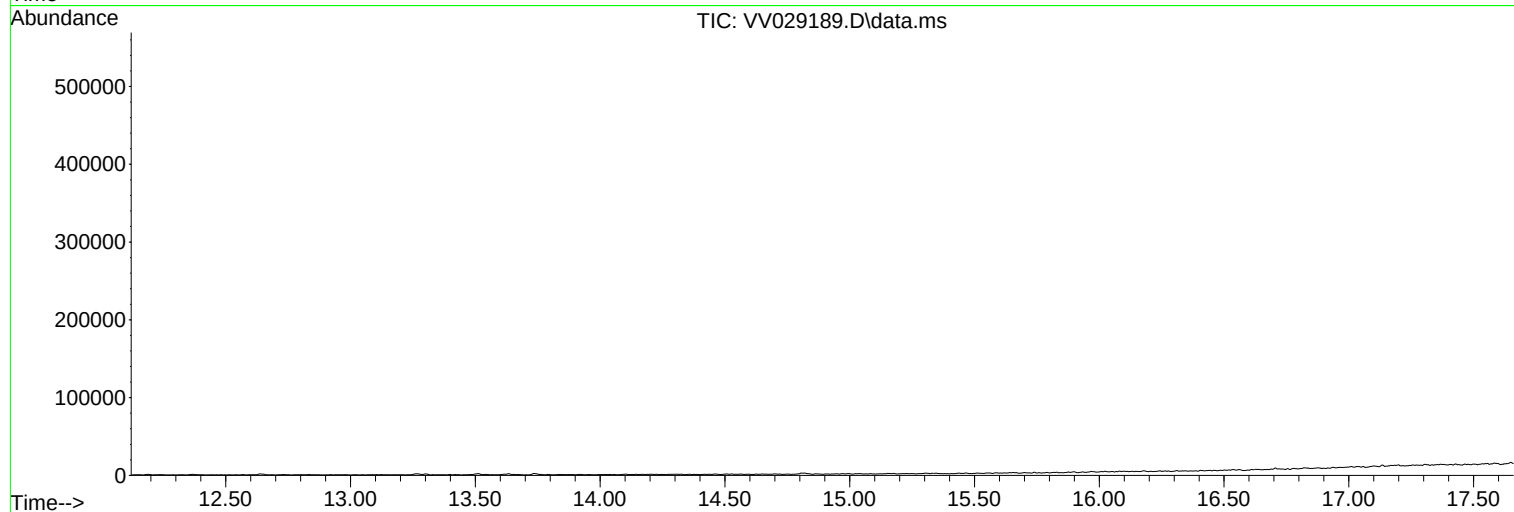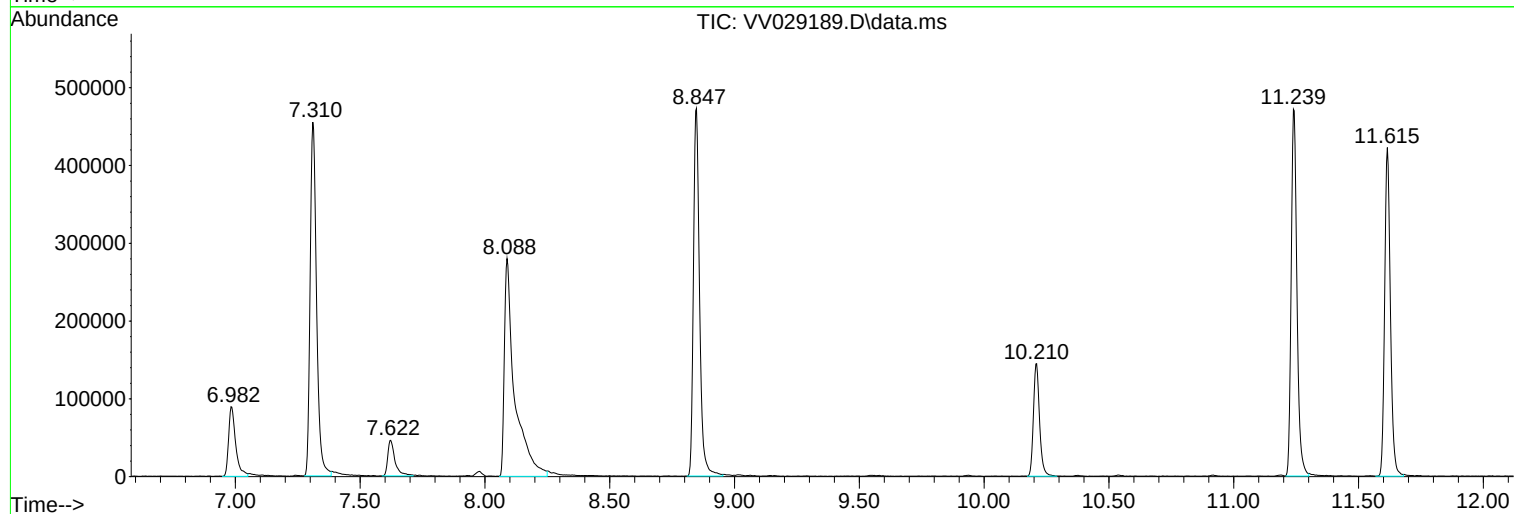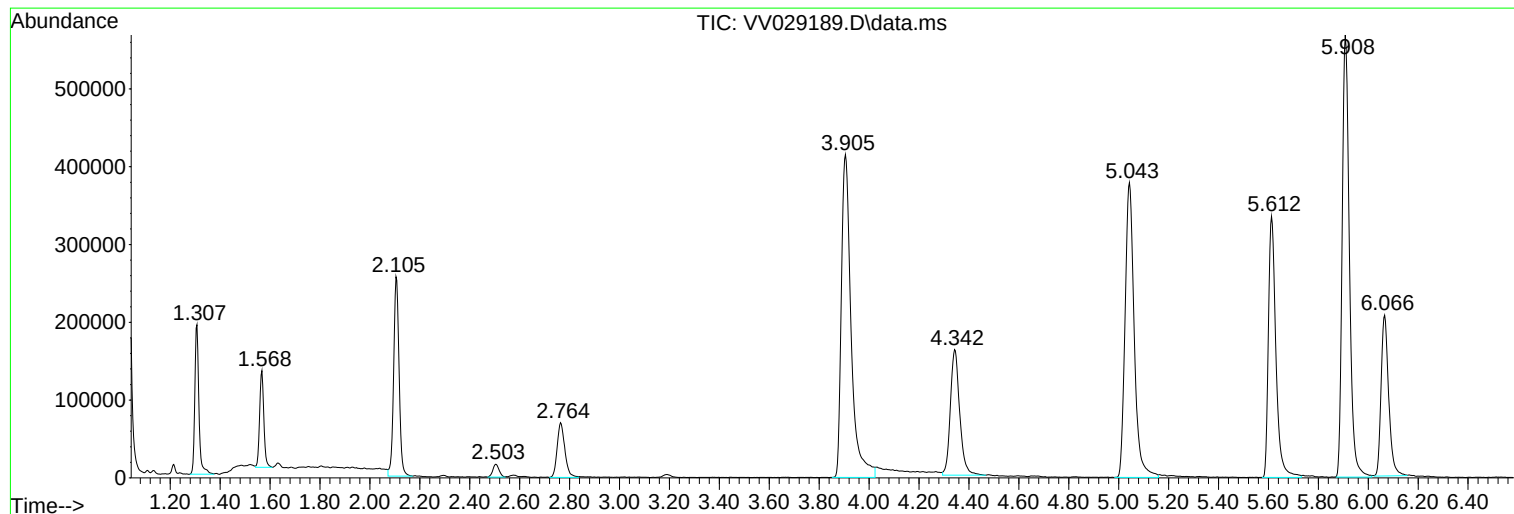

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029189.D
Acq On : 19 Nov 2022 22:53
Operator : SY/MD
Sample : N5648-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029189.D
Acq On : 19 Nov 2022 22:53
Operator : SY/MD
Sample : N5648-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc