

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029190.D
 Acq On : 19 Nov 2022 23:17
 Operator : SY/MD
 Sample : N5648-04DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46D5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB2	168145	182349	11.31%	1.921%
2	1.568	156	164	179	rVB	117636	134073	8.32%	1.413%
3	2.108	322	332	353	rVB	244938	369472	22.91%	3.893%
4	2.506	444	456	471	rBV	18832	33683	2.09%	0.355%
5	2.764	524	536	555	rBV2	36790	72191	4.48%	0.761%
6	3.905	869	891	923	rBV2	613595	1612367	100.00%	16.988%
7	4.342	1013	1027	1062	rVB2	155165	397518	24.65%	4.188%
8	5.043	1229	1245	1280	rBV3	365042	926076	57.44%	9.757%
9	5.612	1410	1422	1452	rBV	326750	679755	42.16%	7.162%
10	5.911	1503	1515	1547	rBV	207234	425664	26.40%	4.485%
11	6.066	1550	1563	1590	rBV	198318	419541	26.02%	4.420%
12	6.985	1836	1849	1874	rBV	84097	169873	10.54%	1.790%
13	7.310	1939	1950	1980	rBV	437208	793256	49.20%	8.358%
14	7.622	2038	2047	2067	rBV2	44746	86494	5.36%	0.911%
15	8.091	2183	2193	2260	rBV	237354	783994	48.62%	8.260%
16	8.847	2416	2428	2469	rBV	463153	800321	49.64%	8.432%
17	10.210	2839	2852	2873	rBV	142521	239176	14.83%	2.520%
18	11.242	3161	3173	3200	rBV	453990	738058	45.77%	7.776%
19	11.615	3276	3289	3313	rBV	383835	627623	38.93%	6.612%




Sum of corrected areas: 9491484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029190.D
Acq On : 19 Nov 2022 23:17
Operator : SY/MD
Sample : N5648-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

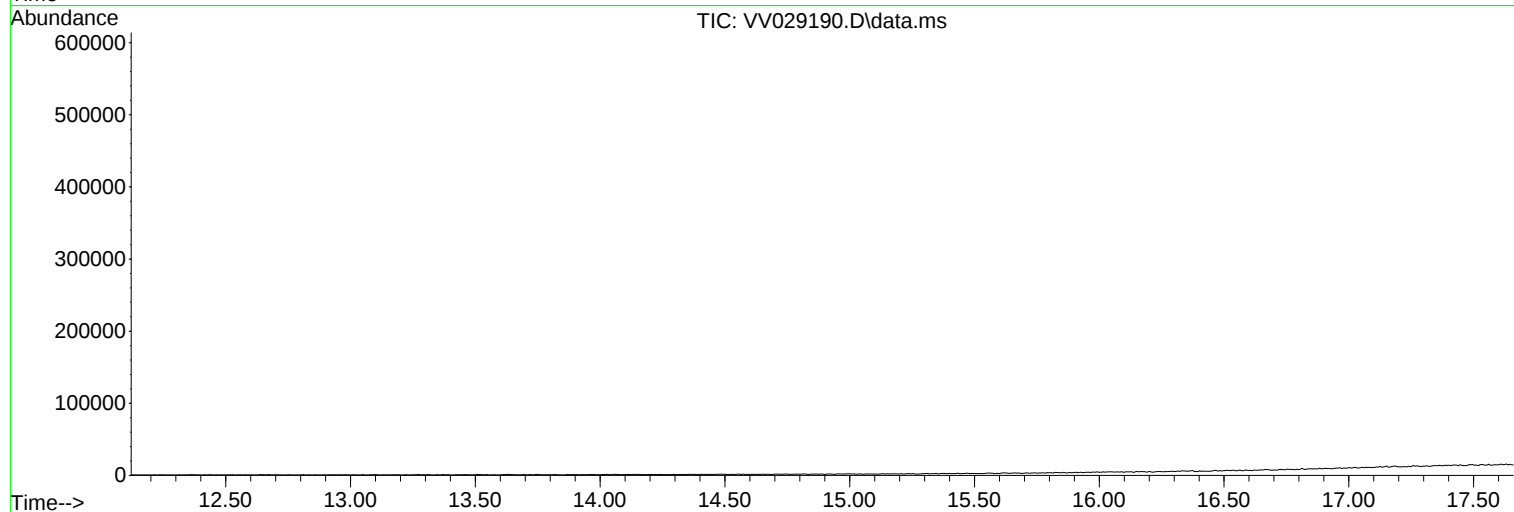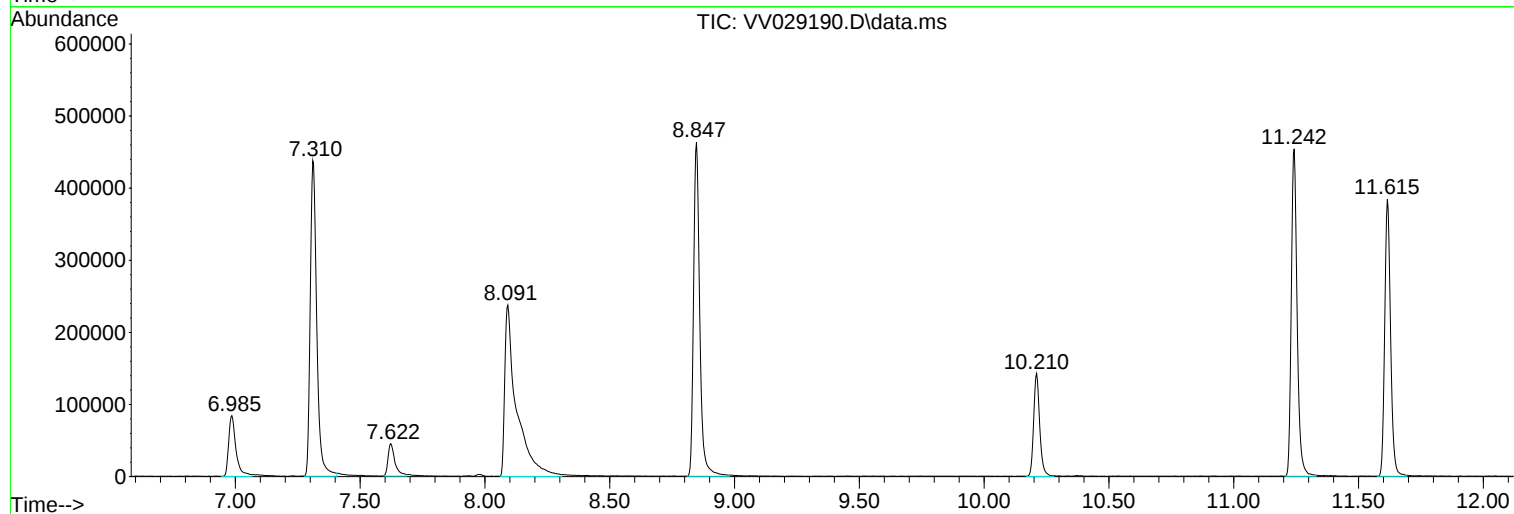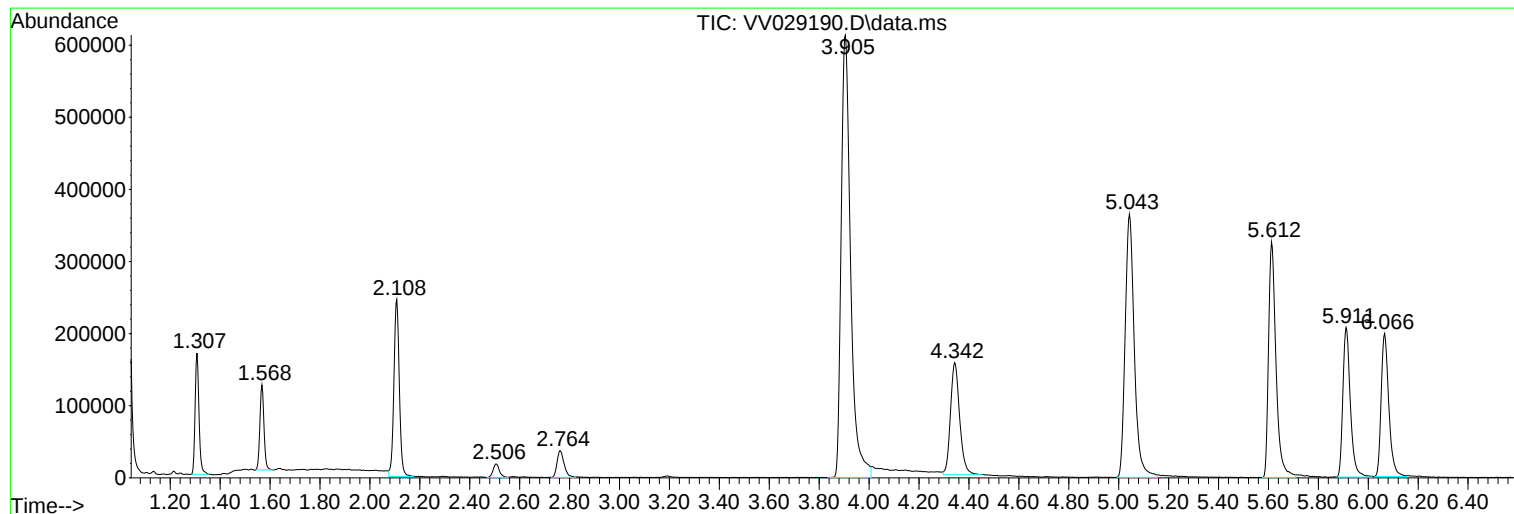

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029190.D
Acq On : 19 Nov 2022 23:17
Operator : SY/MD
Sample : N5648-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029190.D
Acq On : 19 Nov 2022 23:17
Operator : SY/MD
Sample : N5648-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc