

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029191.D
 Acq On : 19 Nov 2022 23:42
 Operator : SY/MD
 Sample : N5648-05DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46D7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	101	rVB2	173561	195205	15.09%	2.080%
2	1.503	127	144	146	rBV	5909	14055	1.09%	0.150%
3	1.564	156	163	175	rBV	115882	133491	10.32%	1.422%
4	2.105	321	331	351	rVB	241122	355864	27.51%	3.792%
5	2.503	444	455	468	rBV2	20165	33758	2.61%	0.360%
6	2.761	521	535	560	rBV3	68879	140168	10.84%	1.493%
7	3.905	876	891	929	rBV	478309	1293372	100.00%	13.780%
8	4.343	1013	1027	1054	rVB	154786	395004	30.54%	4.209%
9	5.043	1229	1245	1278	rBV2	359610	922534	71.33%	9.829%
10	5.613	1407	1422	1450	rBV	339389	704180	54.45%	7.503%
11	5.912	1503	1515	1546	rBV	226406	454794	35.16%	4.846%
12	6.066	1550	1563	1588	rBV	197695	415599	32.13%	4.428%
13	6.985	1837	1849	1877	rBV2	84184	170026	13.15%	1.812%
14	7.310	1936	1950	1986	rBV	442982	793725	61.37%	8.457%
15	7.622	2037	2047	2066	rBV	46246	86731	6.71%	0.924%
16	8.088	2182	2192	2252	rBV	276097	796778	61.60%	8.489%
17	8.844	2414	2427	2453	rBV	484668	819224	63.34%	8.729%
18	10.207	2840	2851	2874	rBV2	138109	236659	18.30%	2.522%
19	11.239	3161	3172	3196	rBV	471503	769148	59.47%	8.195%
20	11.616	3277	3289	3315	rBV	405047	655295	50.67%	6.982%




Sum of corrected areas: 9385610

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029191.D
Acq On : 19 Nov 2022 23:42
Operator : SY/MD
Sample : N5648-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

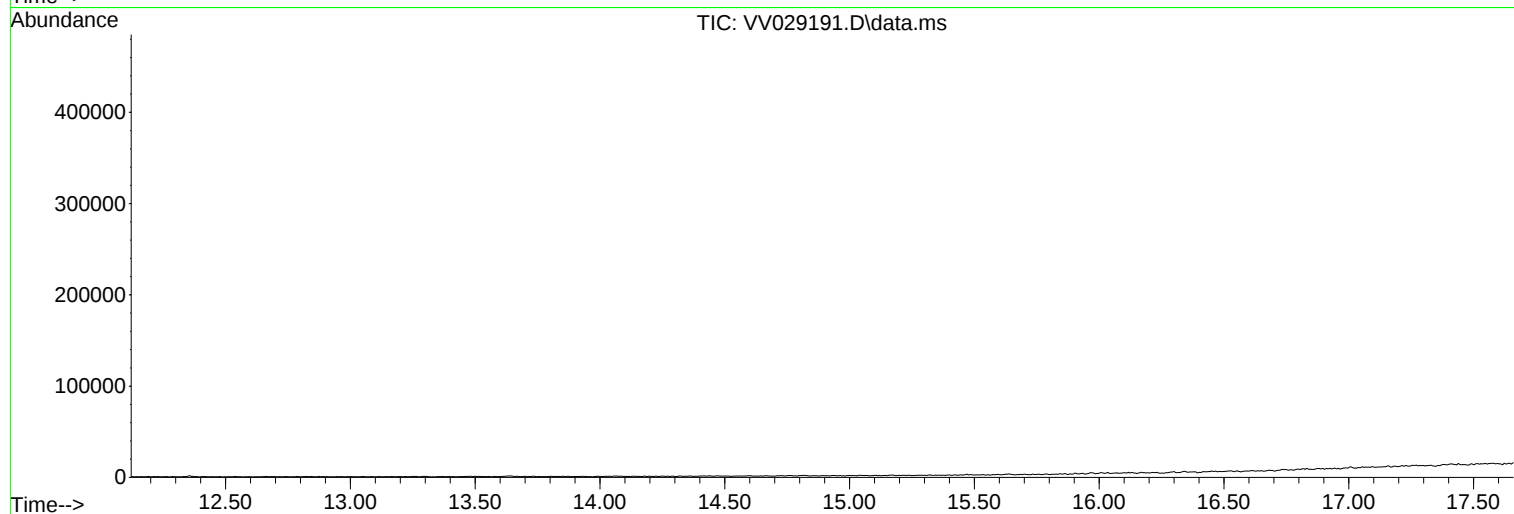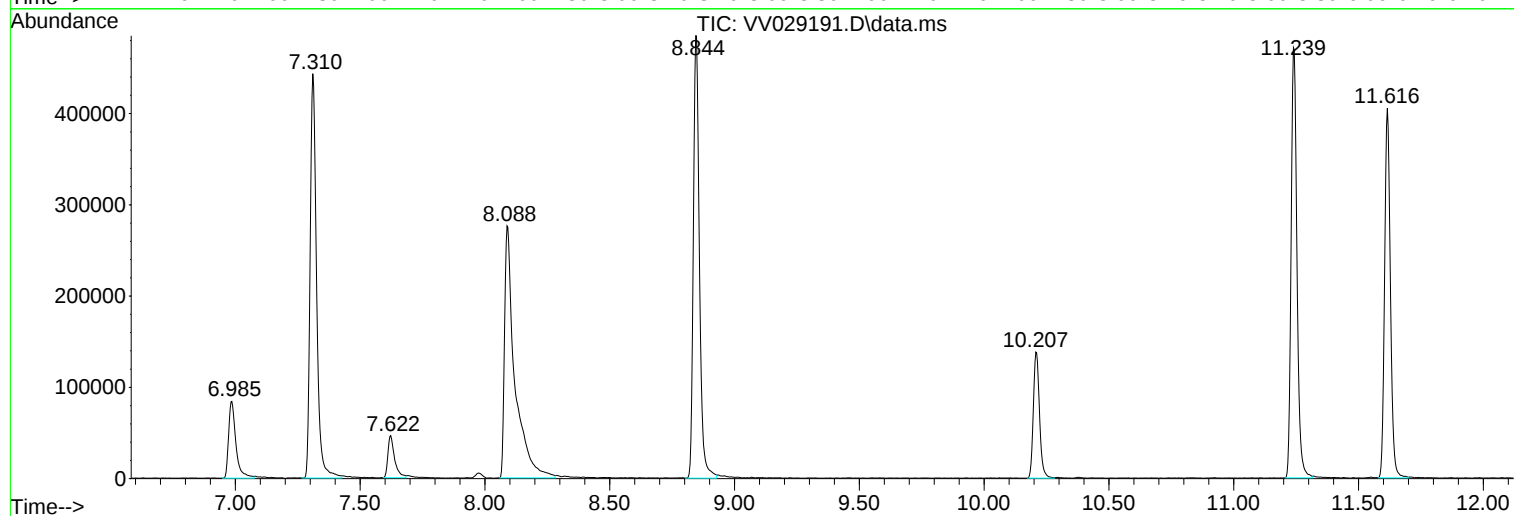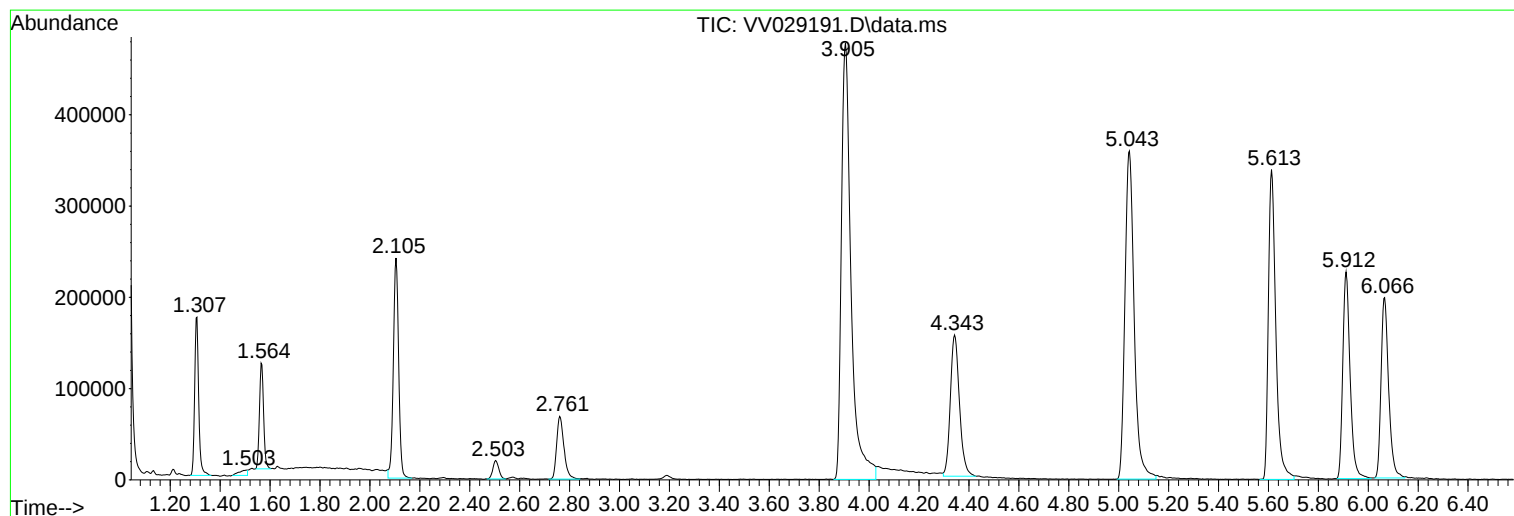

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029191.D
Acq On : 19 Nov 2022 23:42
Operator : SY/MD
Sample : N5648-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029191.D
Acq On : 19 Nov 2022 23:42
Operator : SY/MD
Sample : N5648-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc