

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029192.D
 Acq On : 20 Nov 2022 00:06
 Operator : SY/MD
 Sample : N5648-07DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46E7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	106	rVB2	170003	193039	20.17%	2.179%
2	1.465	117	132	135	rBV	8510	19846	2.07%	0.224%
3	1.568	157	164	180	rVB	122298	140308	14.66%	1.584%
4	2.105	321	331	358	rVB	249331	390015	40.75%	4.403%
5	2.503	445	455	469	rBV2	11901	20614	2.15%	0.233%
6	2.764	520	536	569	rBV	442308	957189	100.00%	10.805%
7	3.905	875	891	930	rBV2	62943	281099	29.37%	3.173%
8	4.342	1012	1027	1056	rVB	156043	397139	41.49%	4.483%
9	5.043	1226	1245	1277	rBV2	372199	943407	98.56%	10.650%
10	5.612	1410	1422	1457	rBV	335037	698221	72.94%	7.882%
11	6.066	1550	1563	1589	rBV	204455	431365	45.07%	4.870%
12	6.985	1838	1849	1868	rBV	85450	169099	17.67%	1.909%
13	7.310	1938	1950	1973	rBV	453901	803919	83.99%	9.075%
14	7.622	2037	2047	2066	rBV2	46785	88046	9.20%	0.994%
15	8.091	2182	2193	2239	rBV2	273700	801635	83.75%	9.049%
16	8.423	2286	2296	2312	rBV3	8209	16769	1.75%	0.189%
17	8.847	2415	2428	2466	rBV	468149	813736	85.01%	9.186%
18	10.210	2840	2852	2872	rBV	147111	245377	25.64%	2.770%
19	11.239	3162	3172	3202	rBV	478602	769088	80.35%	8.682%
20	11.615	3277	3289	3315	rBV	413475	678527	70.89%	7.660%




Sum of corrected areas: 8858438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029192.D
Acq On : 20 Nov 2022 00:06
Operator : SY/MD
Sample : N5648-07DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

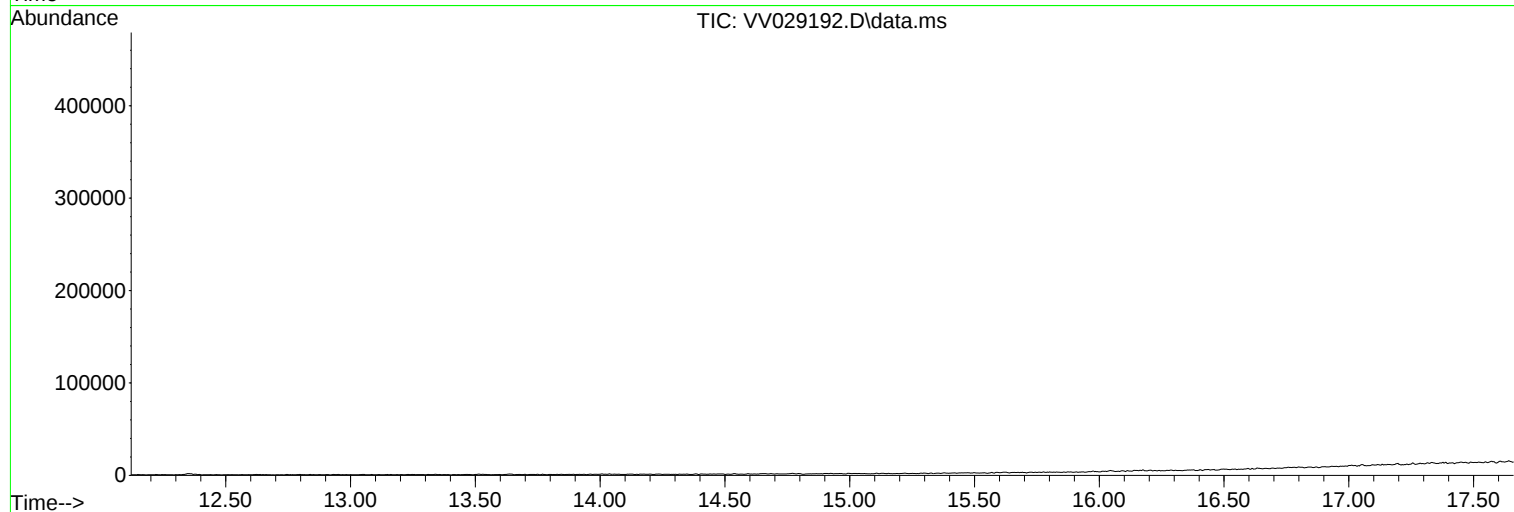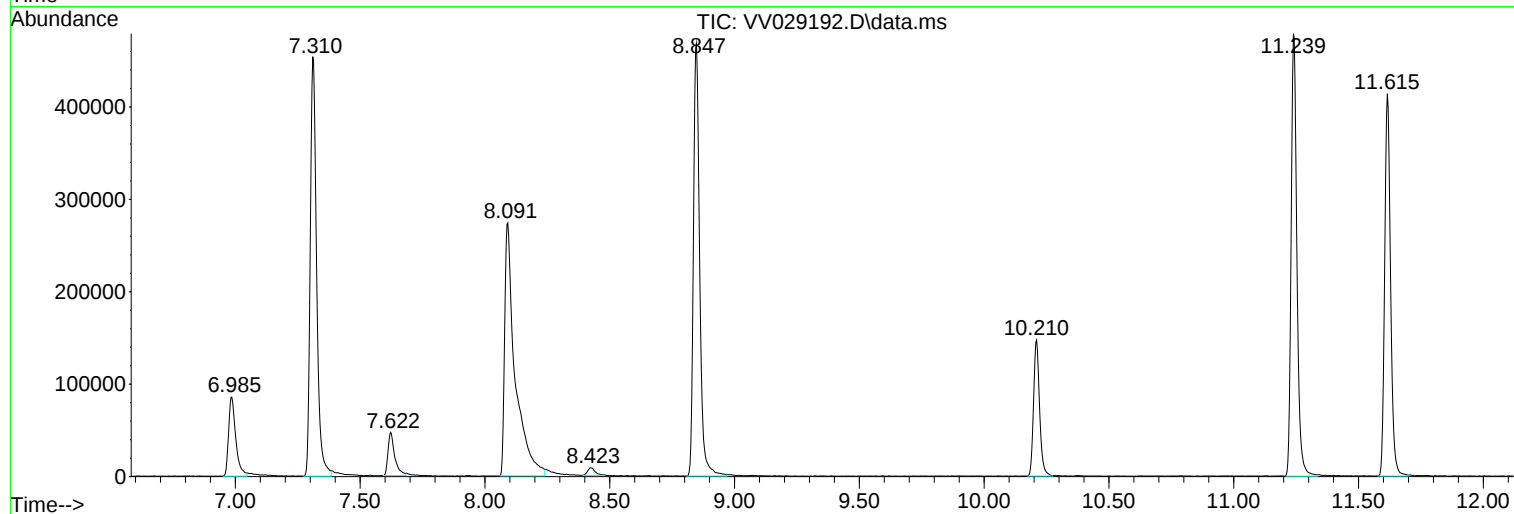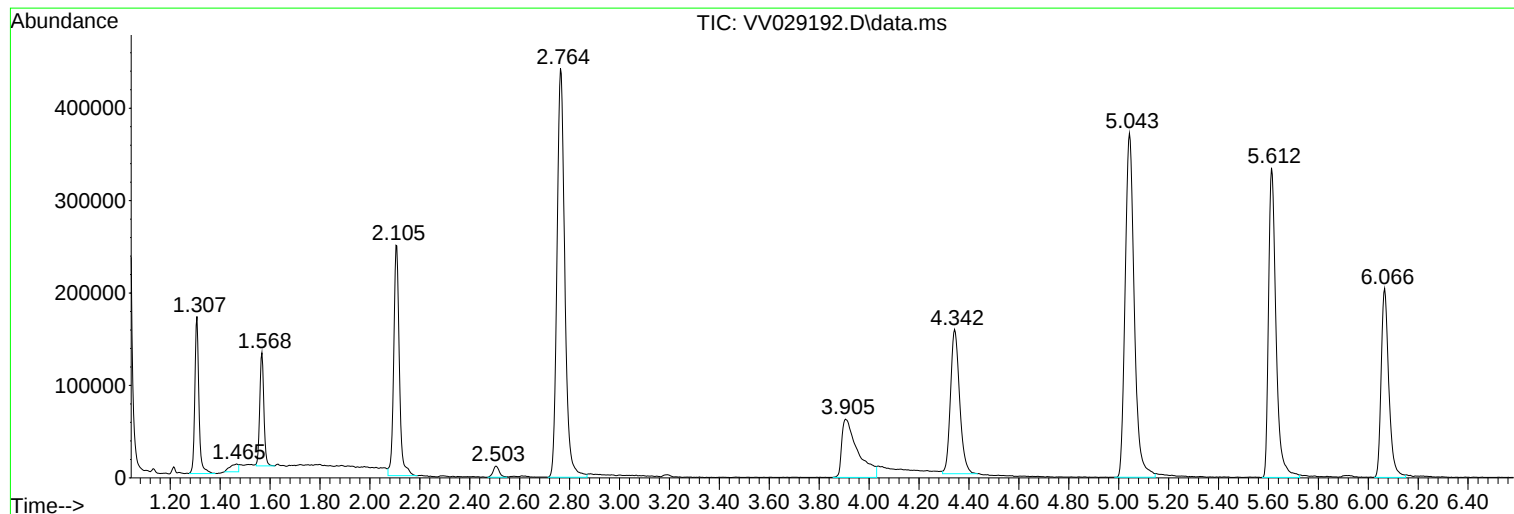

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029192.D
Acq On : 20 Nov 2022 00:06
Operator : SY/MD
Sample : N5648-07DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029192.D
Acq On : 20 Nov 2022 00:06
Operator : SY/MD
Sample : N5648-07DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc