

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029193.D
 Acq On : 20 Nov 2022 00:31
 Operator : SY/MD
 Sample : N5648-11DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46E9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	73	84	103	rBV2	275664	330330	33.84%	3.877%
2	1.426	109	120	121	rBV	29216	40284	4.13%	0.473%
3	1.568	157	164	178	rVB	123498	147954	15.16%	1.736%
4	1.632	180	184	195	rVB4	12674	16995	1.74%	0.199%
5	2.108	322	332	350	rVB	250667	368504	37.75%	4.325%
6	2.506	444	456	469	rBV3	13398	22412	2.30%	0.263%
7	2.764	524	536	553	rBV4	48359	96582	9.89%	1.133%
8	3.188	656	668	682	rBV2	9712	22974	2.35%	0.270%
9	3.902	873	890	935	rBV4	160406	575633	58.96%	6.756%
10	4.342	1011	1027	1060	rBV	161211	401226	41.10%	4.709%
11	5.043	1228	1245	1281	rBV2	376710	976229	100.00%	11.457%
12	5.612	1410	1422	1462	rBV	330543	699468	71.65%	8.209%
13	6.066	1550	1563	1588	rBV	206167	433219	44.38%	5.084%
14	6.985	1838	1849	1872	rBV	86683	170621	17.48%	2.002%
15	7.310	1937	1950	1986	rBV	448027	816982	83.69%	9.588%
16	7.622	2037	2047	2070	rBV	46512	90385	9.26%	1.061%
17	8.088	2181	2192	2233	rBV	336642	824977	84.51%	9.682%
18	8.847	2416	2428	2459	rBV	481053	813768	83.36%	9.550%
19	10.210	2839	2852	2872	rBV	151239	247730	25.38%	2.907%
20	11.242	3161	3173	3195	rBV	462032	758314	77.68%	8.899%
21	11.615	3278	3289	3311	rBV	409140	666329	68.26%	7.820%




Sum of corrected areas: 8520916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029193.D
Acq On : 20 Nov 2022 00:31
Operator : SY/MD
Sample : N5648-11DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

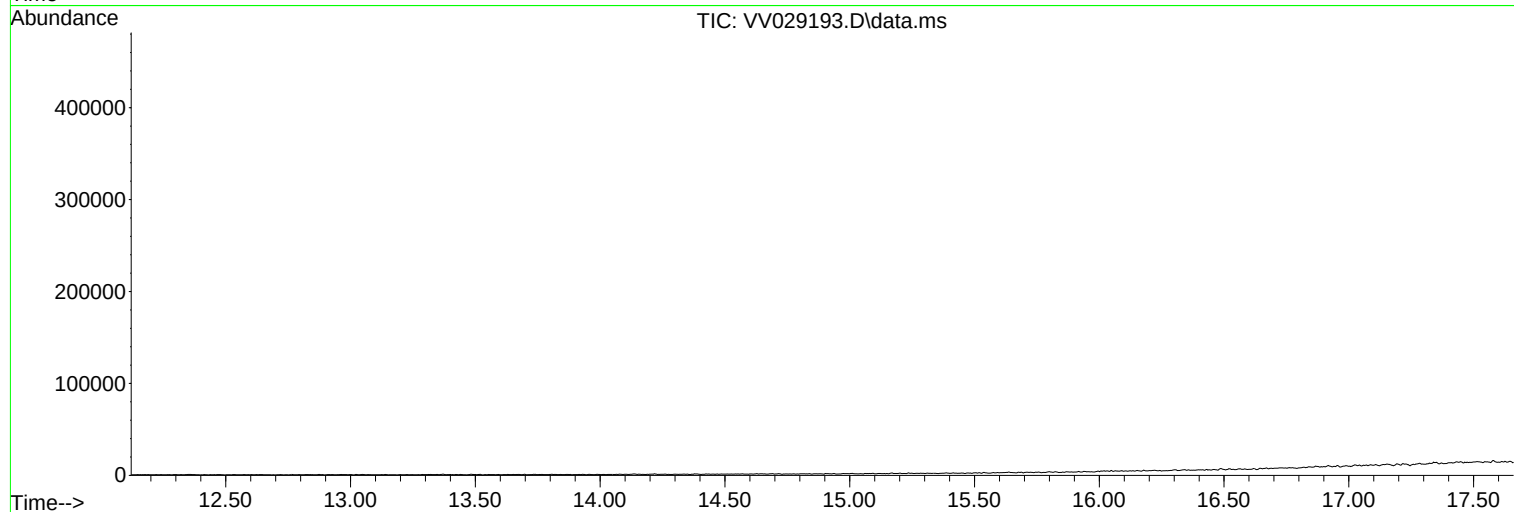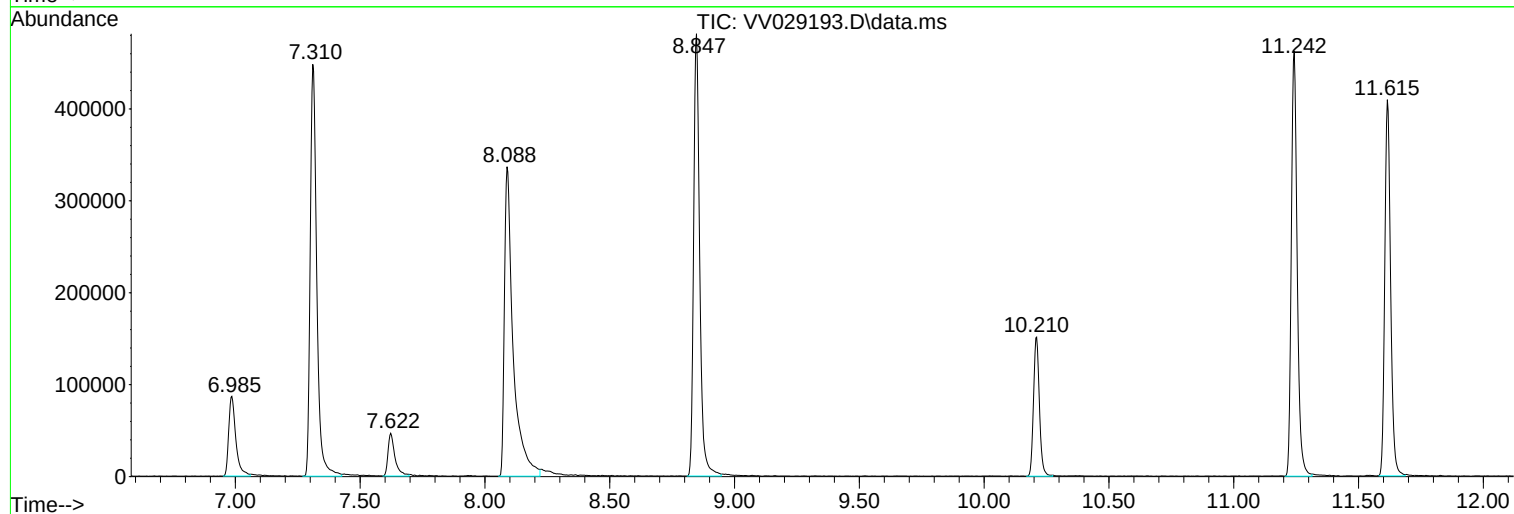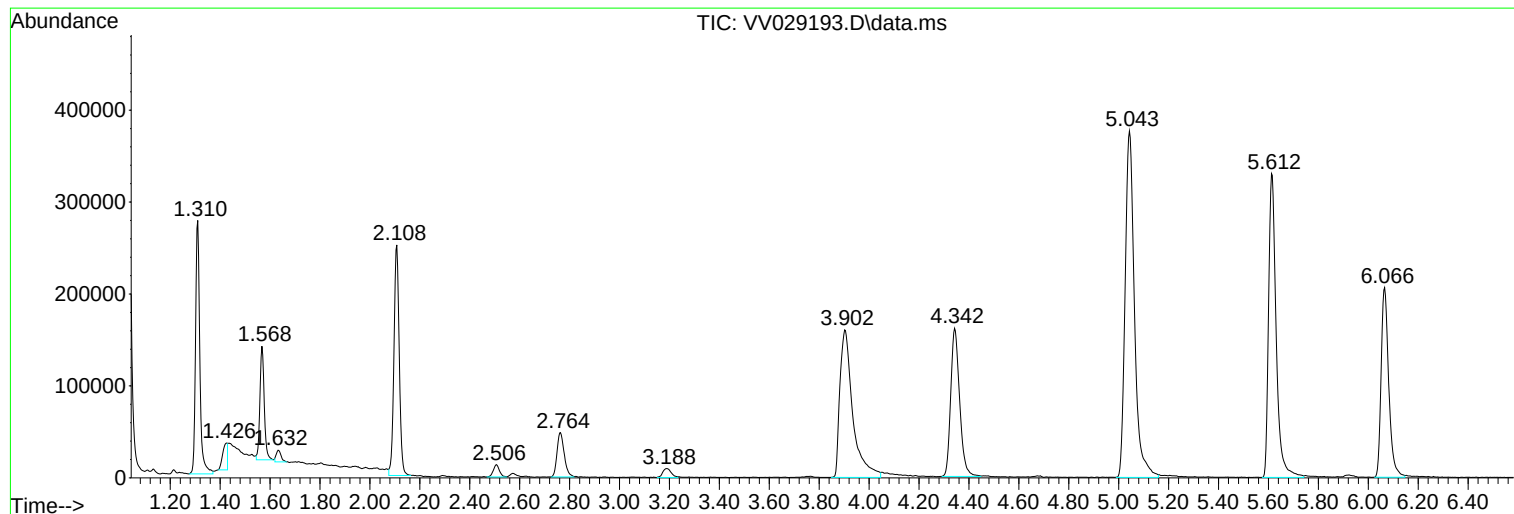

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029193.D
Acq On : 20 Nov 2022 00:31
Operator : SY/MD
Sample : N5648-11DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029193.D
Acq On : 20 Nov 2022 00:31
Operator : SY/MD
Sample : N5648-11DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc