

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029195.D
 Acq On : 20 Nov 2022 01:20
 Operator : SY/MD
 Sample : N5648-13DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46E0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	48	54	59	rBV3	10692	10028	1.07%	0.118%
2	1.307	74	83	102	rBV2	181216	203115	21.74%	2.396%
3	1.452	113	128	129	rBV4	8672	16165	1.73%	0.191%
4	1.568	156	164	175	rBV	116044	132733	14.21%	1.566%
5	2.108	322	332	353	rVB	244563	367980	39.39%	4.342%
6	2.506	445	456	469	rBV	33222	54812	5.87%	0.647%
7	2.760	522	535	560	rBV3	123642	255074	27.30%	3.009%
8	3.905	877	891	934	rBV2	222512	685807	73.41%	8.091%
9	4.342	1013	1027	1059	rVB2	156423	403778	43.22%	4.764%
10	5.043	1228	1245	1286	rBV2	361900	934266	100.00%	11.023%
11	5.612	1410	1422	1450	rBV	320320	668611	71.57%	7.888%
12	5.918	1506	1517	1542	rVB4	19252	44076	4.72%	0.520%
13	6.066	1549	1563	1593	rBV	199626	426687	45.67%	5.034%
14	6.985	1838	1849	1880	rBV	83917	168621	18.05%	1.989%
15	7.310	1939	1950	1984	rBV	426948	792823	84.86%	9.354%
16	7.622	2038	2047	2068	rBV	43569	85310	9.13%	1.007%
17	8.091	2182	2193	2254	rBV	246144	807608	86.44%	9.528%
18	8.847	2417	2428	2460	rBV	462364	790046	84.56%	9.321%
19	10.210	2841	2852	2880	rBV	143603	243064	26.02%	2.868%
20	11.242	3161	3173	3198	rBV	456095	733198	78.48%	8.650%
21	11.615	3277	3289	3318	rBV	397242	652006	69.79%	7.693%




Sum of corrected areas: 8475808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029195.D
Acq On : 20 Nov 2022 01:20
Operator : SY/MD
Sample : N5648-13DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

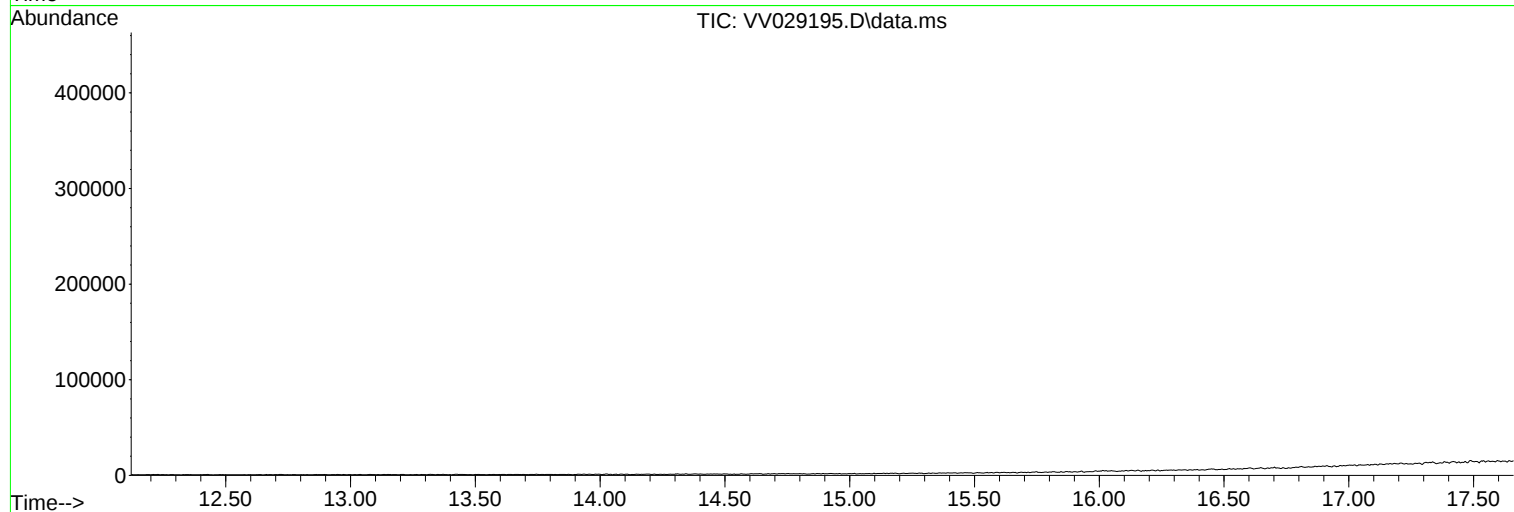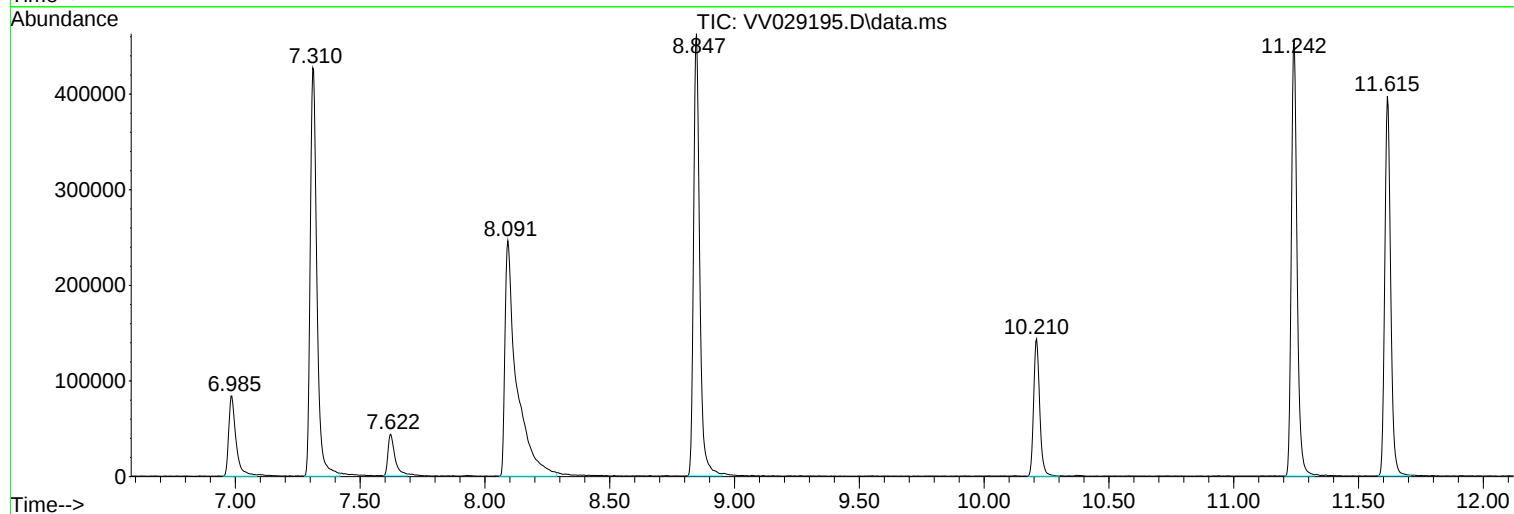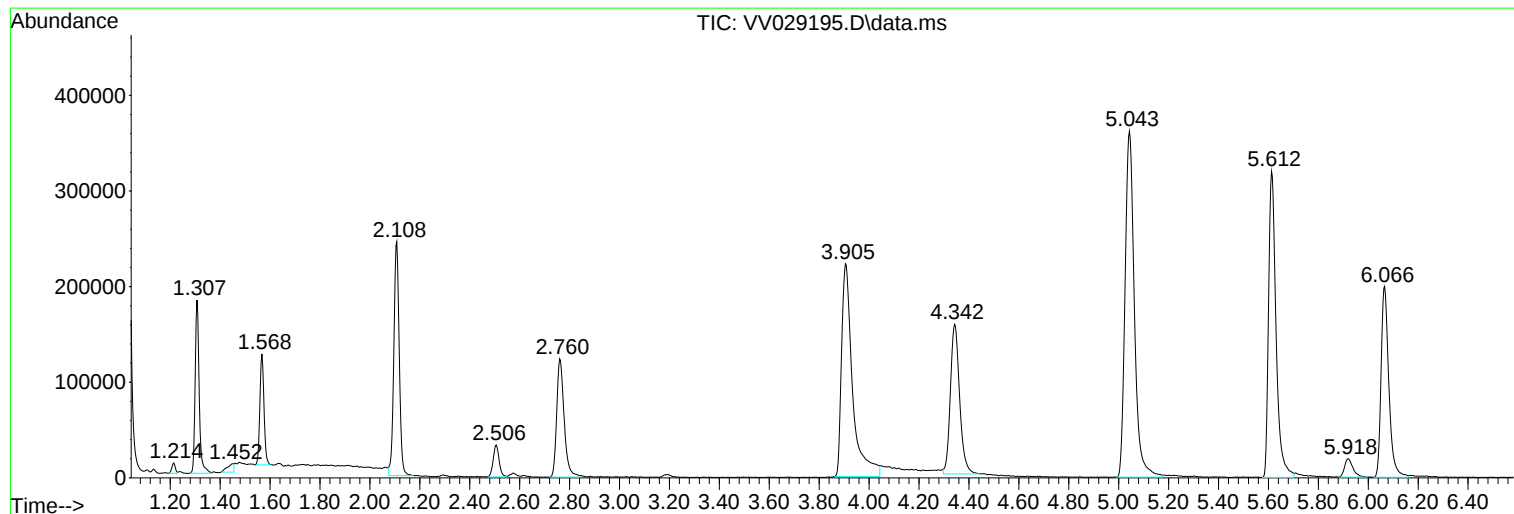

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029195.D
Acq On : 20 Nov 2022 01:20
Operator : SY/MD
Sample : N5648-13DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029195.D
Acq On : 20 Nov 2022 01:20
Operator : SY/MD
Sample : N5648-13DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc