

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029197.D
 Acq On : 20 Nov 2022 02:09
 Operator : SY/MD
 Sample : N5648-15DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46E2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	72	83	104	rVB2	154089	178321	19.68%	2.005%
2	1.568	157	164	177	rVB	115761	134265	14.82%	1.510%
3	2.105	322	331	354	rVB	238394	366817	40.49%	4.125%
4	2.503	446	455	468	rBV3	12256	21030	2.32%	0.236%
5	2.764	521	536	565	rBV2	397955	856967	94.59%	9.637%
6	3.905	877	891	929	rBV2	259785	767554	84.72%	8.631%
7	4.342	1013	1027	1049	rVB	151305	374996	41.39%	4.217%
8	5.043	1228	1245	1274	rBV2	360663	905948	100.00%	10.188%
9	5.612	1410	1422	1454	rBV	319310	664376	73.33%	7.471%
10	5.918	1504	1517	1535	rBV4	15759	34990	3.86%	0.393%
11	6.066	1551	1563	1591	rBV	197236	416427	45.97%	4.683%
12	6.985	1838	1849	1881	rBV	79748	164000	18.10%	1.844%
13	7.310	1939	1950	1973	rBV	424926	766576	84.62%	8.620%
14	7.622	2037	2047	2073	rBV	43981	87490	9.66%	0.984%
15	8.088	2182	2192	2243	rBV2	250992	776401	85.70%	8.731%
16	8.847	2417	2428	2453	rBV	462157	775456	85.60%	8.720%
17	10.210	2840	2852	2876	rBV	140331	237069	26.17%	2.666%
18	11.239	3162	3172	3195	rBV	445557	720881	79.57%	8.107%
19	11.615	3277	3289	3316	rBV	397820	642944	70.97%	7.230%




Sum of corrected areas: 8892508

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029197.D
Acq On : 20 Nov 2022 02:09
Operator : SY/MD
Sample : N5648-15DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

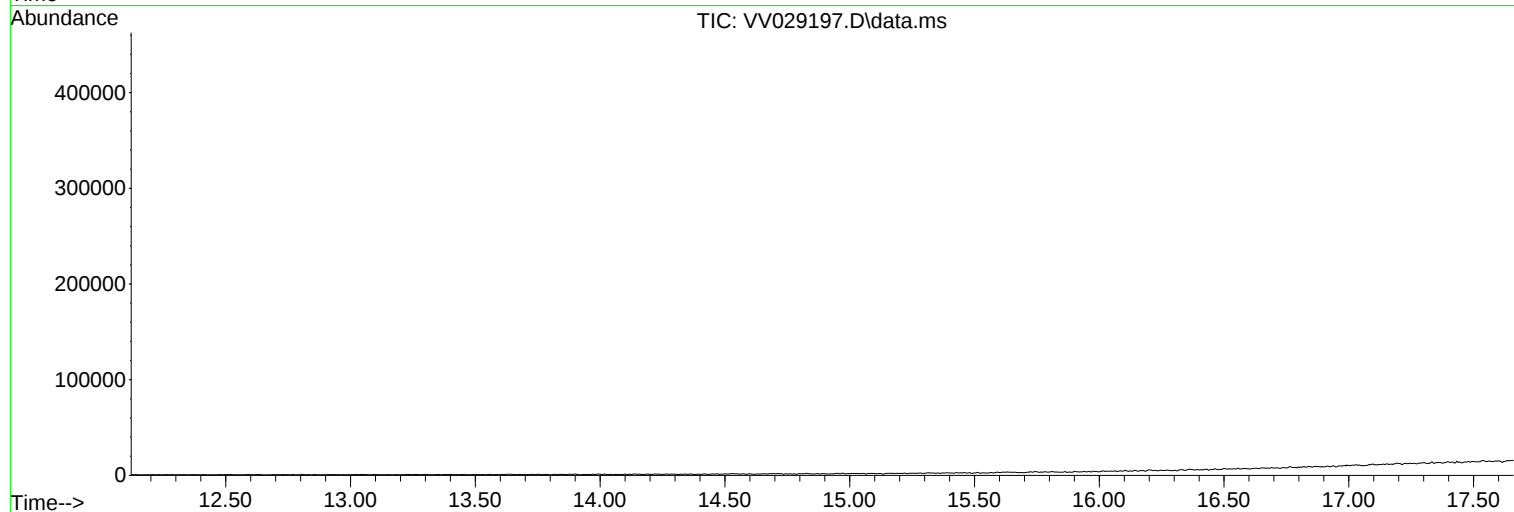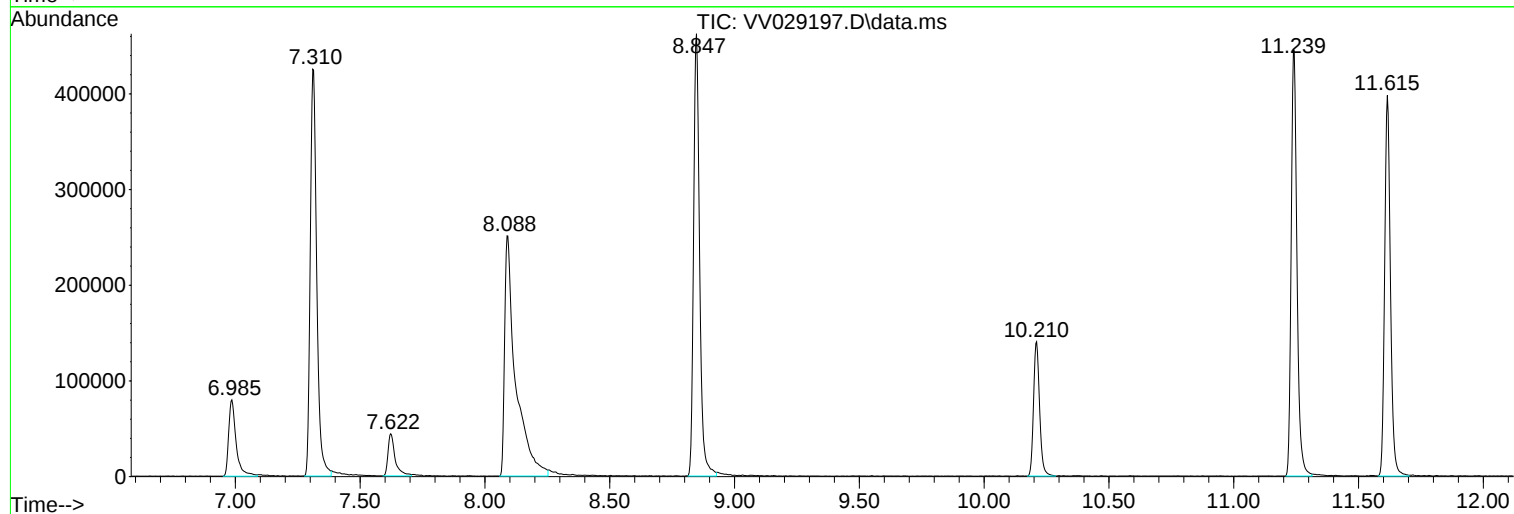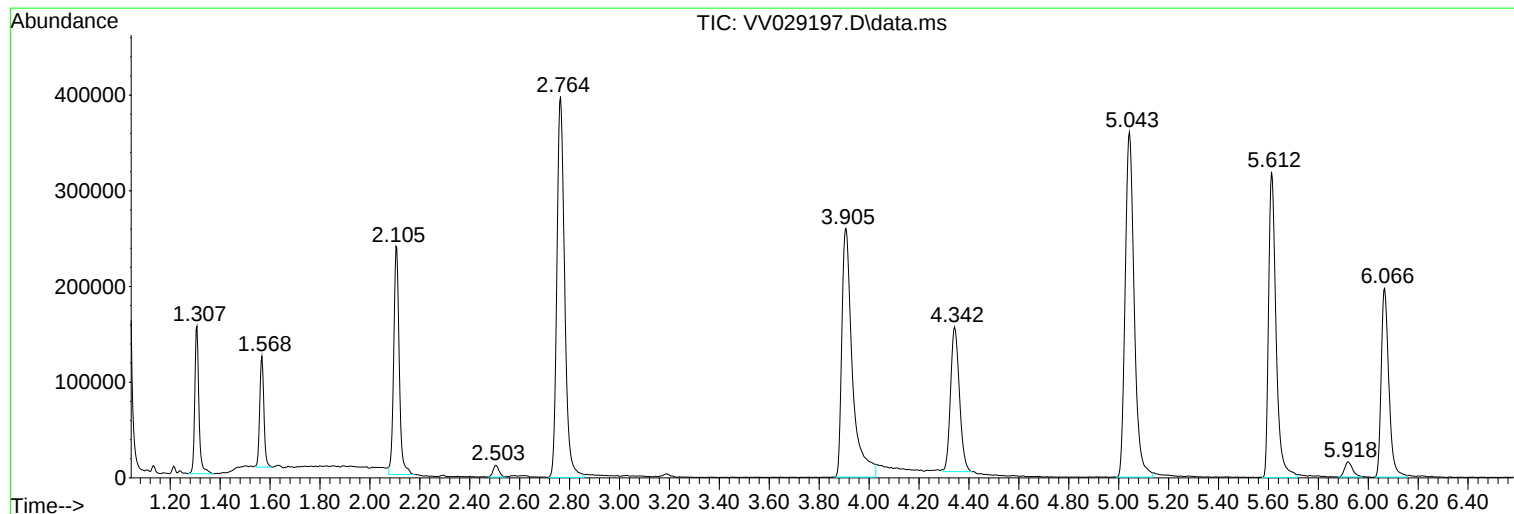

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029197.D
Acq On : 20 Nov 2022 02:09
Operator : SY/MD
Sample : N5648-15DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029197.D
Acq On : 20 Nov 2022 02:09
Operator : SY/MD
Sample : N5648-15DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46E2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
