

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029198.D
 Acq On : 20 Nov 2022 02:33
 Operator : SY/MD
 Sample : N5648-16DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46F5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	101	rBV2	170258	190826	21.64%	2.426%
2	1.475	123	135	138	rBV2	5068	9205	1.04%	0.117%
3	1.568	156	164	175	rBV	113148	129583	14.69%	1.647%
4	2.105	321	331	350	rVB	231514	346031	39.24%	4.399%
5	2.503	446	455	471	rVB	27493	47475	5.38%	0.604%
6	2.764	525	536	551	rBV4	11855	22599	2.56%	0.287%
7	3.905	872	891	923	rBV3	204426	608300	68.98%	7.734%
8	4.343	1013	1027	1050	rVB	150127	370851	42.05%	4.715%
9	5.044	1229	1245	1270	rBV2	349063	881906	100.00%	11.212%
10	5.613	1410	1422	1457	rBV	334390	697896	79.13%	8.873%
11	6.066	1549	1563	1589	rBV	193147	406875	46.14%	5.173%
12	6.986	1838	1849	1868	rBV2	79863	157798	17.89%	2.006%
13	7.310	1938	1950	1982	rBV	420248	763050	86.52%	9.701%
14	7.622	2037	2047	2066	rBV	42097	80963	9.18%	1.029%
15	8.088	2180	2192	2248	rBV	236104	750083	85.05%	9.536%
16	8.847	2415	2428	2450	rBV	472046	803544	91.11%	10.216%
17	10.211	2840	2852	2876	rBV	136933	230744	26.16%	2.934%
18	11.243	3162	3173	3205	rBV	450189	737656	83.64%	9.378%
19	11.616	3277	3289	3309	rBV	378476	630307	71.47%	8.013%




Sum of corrected areas: 7865692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029198.D
Acq On : 20 Nov 2022 02:33
Operator : SY/MD
Sample : N5648-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46F5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

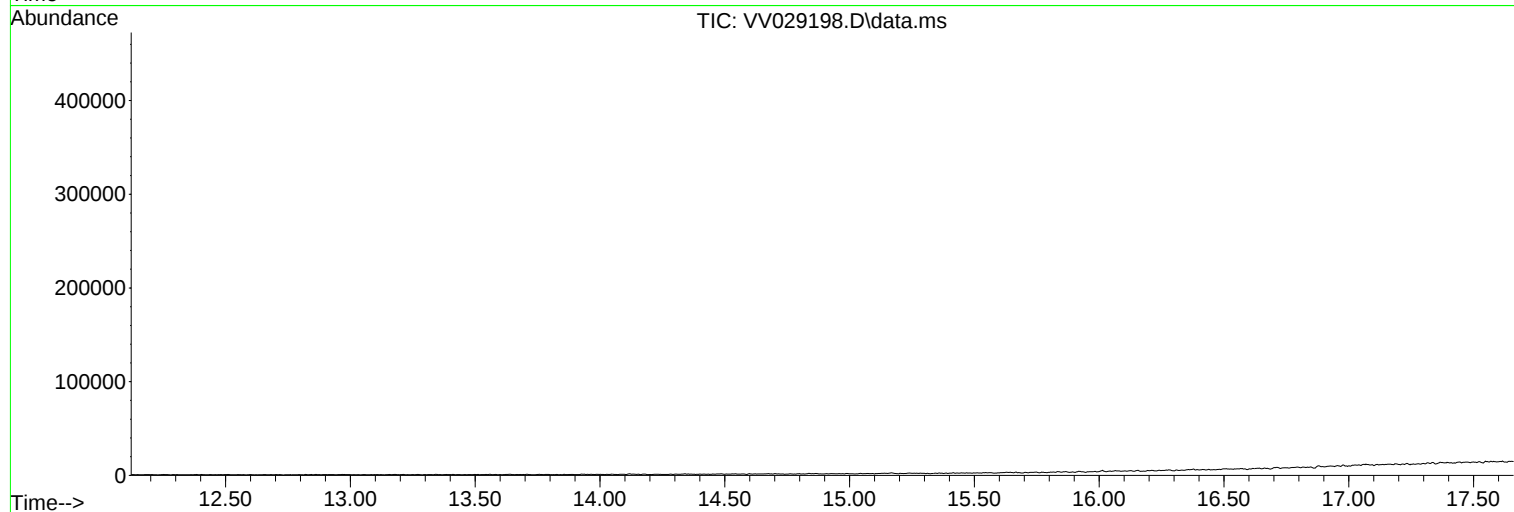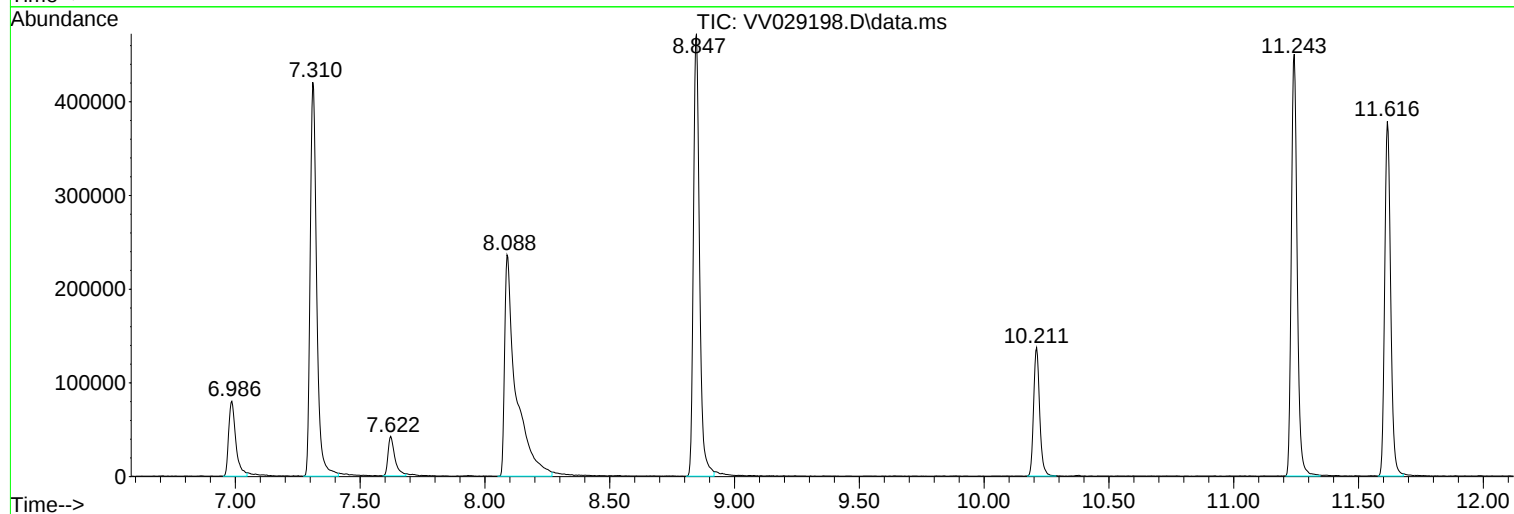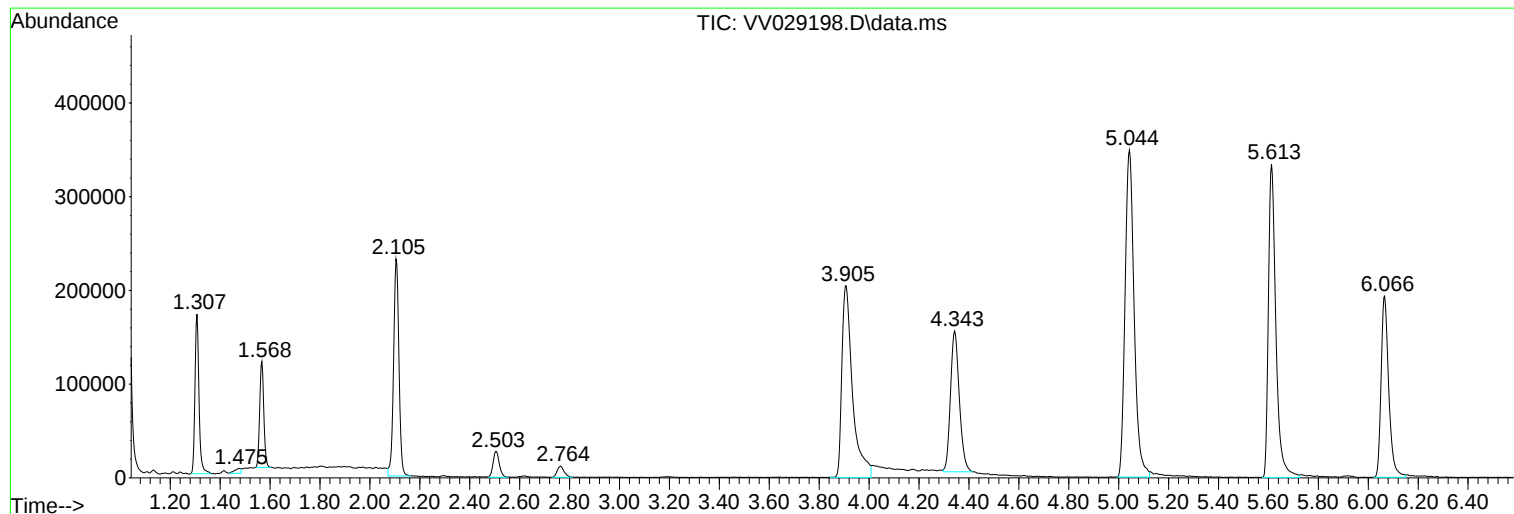

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029198.D
Acq On : 20 Nov 2022 02:33
Operator : SY/MD
Sample : N5648-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46F5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029198.D
Acq On : 20 Nov 2022 02:33
Operator : SY/MD
Sample : N5648-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46F5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc