

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029200.D
 Acq On : 20 Nov 2022 03:22
 Operator : SY/MD
 Sample : N5651-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1G4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	38	rVB2	19344	19123	2.12%	0.244%
2	1.307	74	83	98	rBV	136876	149030	16.49%	1.904%
3	1.452	113	128	129	rBV6	17403	28328	3.14%	0.362%
4	1.568	157	164	180	rVB	119745	138852	15.37%	1.774%
5	2.108	322	332	349	rVB	239114	354820	39.27%	4.532%
6	2.764	521	536	565	rBV	94590	210335	23.28%	2.687%
7	3.899	878	889	913	rBV	63475	222470	24.62%	2.842%
8	4.342	1009	1027	1052	rBV	147803	381158	42.19%	4.868%
9	5.043	1229	1245	1269	rBV2	356255	903511	100.00%	11.540%
10	5.612	1410	1422	1450	rBV	318731	671035	74.27%	8.571%
11	5.921	1507	1518	1541	rVB4	13687	32255	3.57%	0.412%
12	6.066	1550	1563	1588	rBV	199210	419935	46.48%	5.364%
13	6.985	1839	1849	1875	rBV2	82133	162995	18.04%	2.082%
14	7.310	1939	1950	1975	rBV	428798	777388	86.04%	9.929%
15	7.622	2036	2047	2077	rBV	44016	88224	9.76%	1.127%
16	7.972	2146	2156	2177	rVB	36953	66570	7.37%	0.850%
17	8.088	2182	2192	2231	rBV2	303725	788701	87.29%	10.074%
18	8.847	2417	2428	2462	rBV	465630	798244	88.35%	10.196%
19	10.210	2840	2852	2873	rBV	146059	238819	26.43%	3.050%
20	11.242	3161	3173	3195	rBV	455194	731426	80.95%	9.342%
21	11.615	3277	3289	3318	rBV	394615	645876	71.49%	8.250%




Sum of corrected areas: 7829095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029200.D
Acq On : 20 Nov 2022 03:22
Operator : SY/MD
Sample : N5651-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

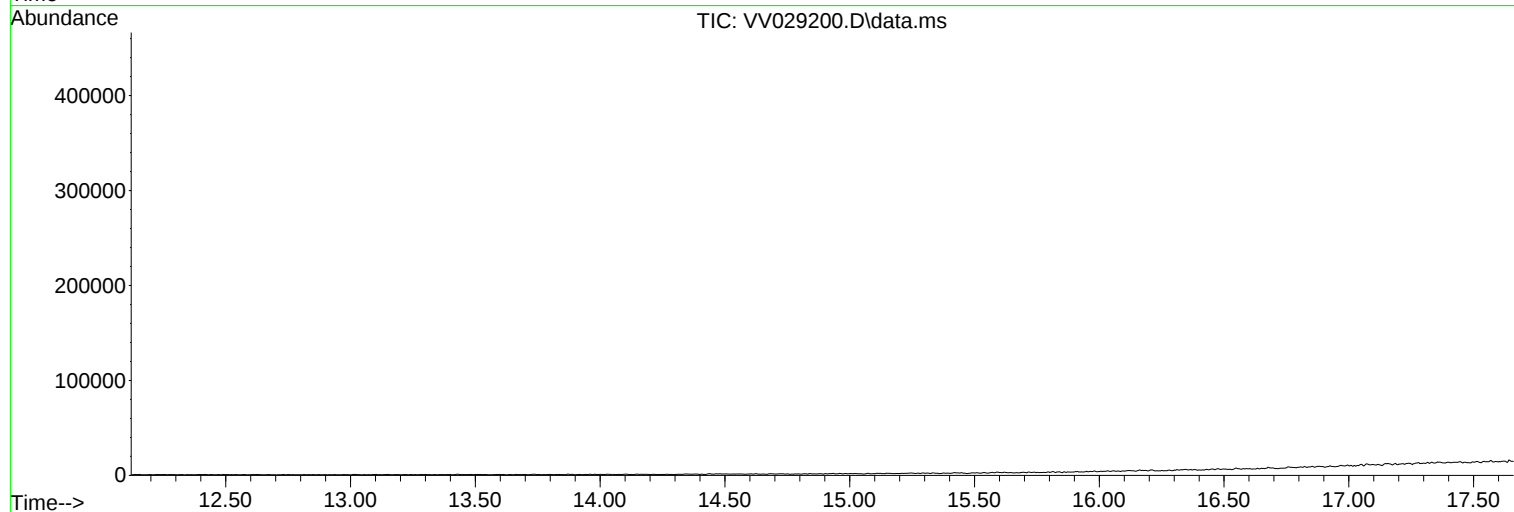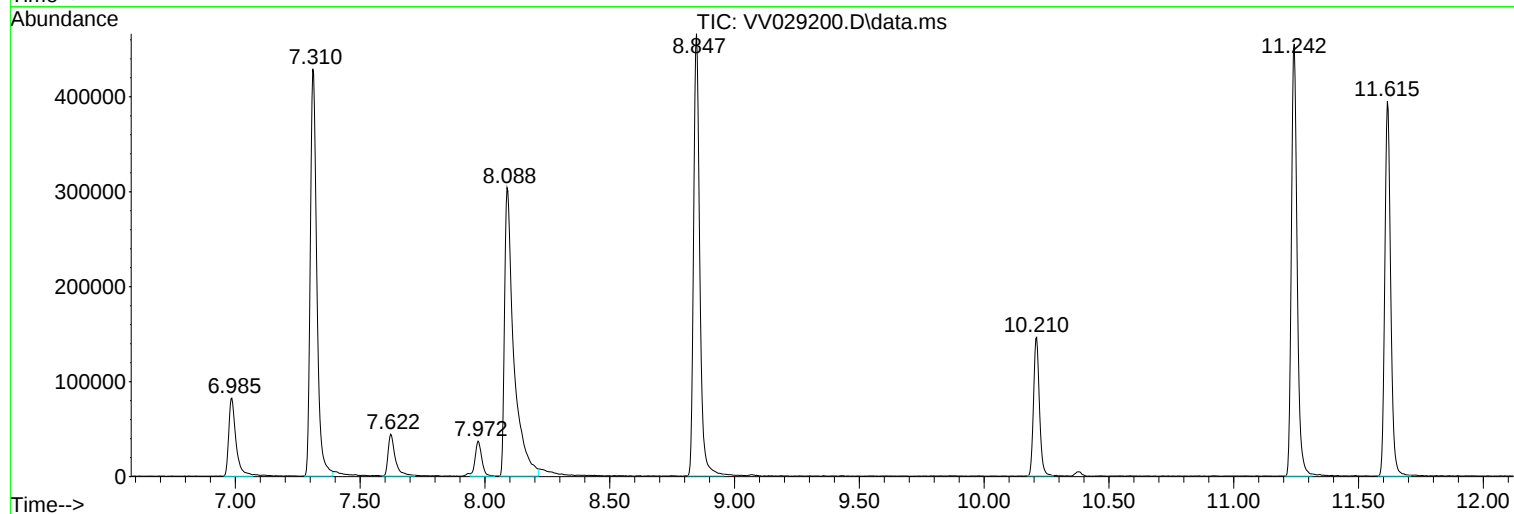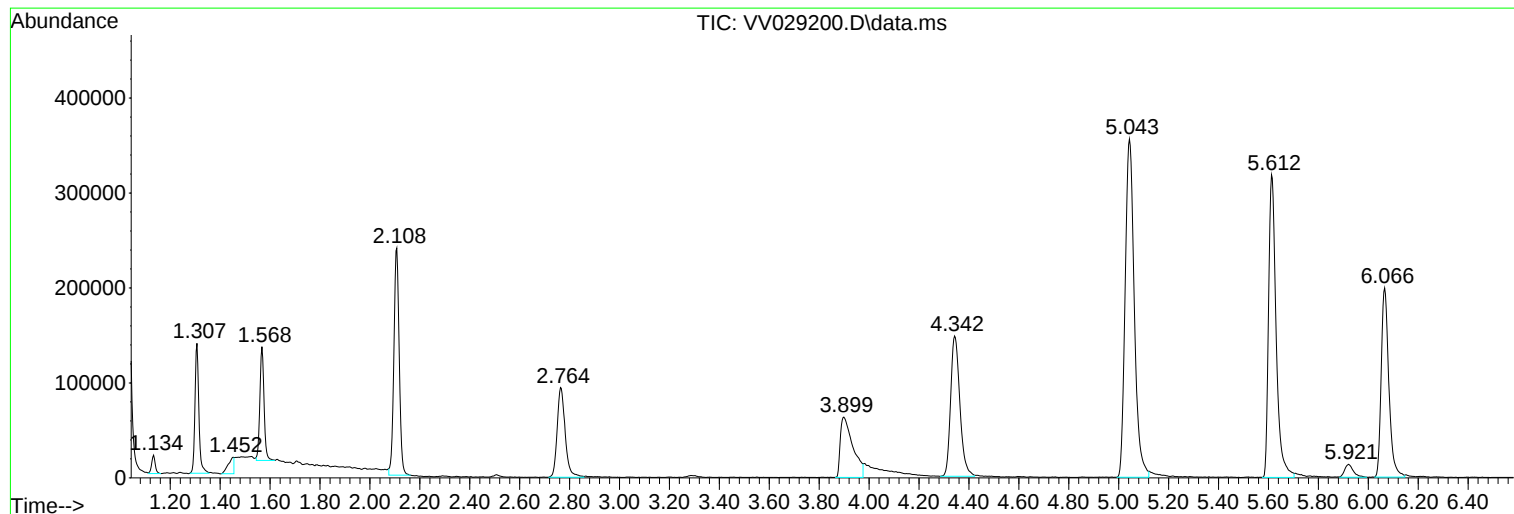

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029200.D
Acq On : 20 Nov 2022 03:22
Operator : SY/MD
Sample : N5651-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029200.D
Acq On : 20 Nov 2022 03:22
Operator : SY/MD
Sample : N5651-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc