

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
 Data File : VV029201.D
 Acq On : 20 Nov 2022 03:47
 Operator : SY/MD
 Sample : N5651-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1G5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB	138008	151265	2.83%	1.067%
2	1.452	112	128	133	rBV2	20357	55592	1.04%	0.392%
3	1.568	157	164	176	rVB	120227	139627	2.61%	0.985%
4	1.751	211	221	247	rVB	4047370	5341637	100.00%	37.690%
5	2.108	321	332	350	rVB3	314205	528443	9.89%	3.729%
6	3.185	652	667	688	rBV	100533	218360	4.09%	1.541%
7	3.899	869	889	918	rBV2	102398	392312	7.34%	2.768%
8	4.342	1008	1027	1059	rBV	152416	393172	7.36%	2.774%
9	5.043	1229	1245	1278	rBV2	357729	910430	17.04%	6.424%
10	5.612	1410	1422	1454	rBV	319671	665321	12.46%	4.694%
11	5.911	1502	1515	1539	rBV	317856	648061	12.13%	4.573%
12	6.066	1550	1563	1589	rBV	200165	413960	7.75%	2.921%
13	6.985	1835	1849	1875	rBV	82436	167448	3.13%	1.182%
14	7.310	1938	1950	1976	rBV	429253	776885	14.54%	5.482%
15	7.622	2037	2047	2067	rBV	44609	86020	1.61%	0.607%
16	8.088	2182	2192	2254	rBV	299424	801003	15.00%	5.652%
17	8.847	2417	2428	2460	rBV	459876	779088	14.59%	5.497%
18	10.207	2838	2851	2873	rBV	144104	236915	4.44%	1.672%
19	10.374	2890	2903	2918	rBV2	58843	100942	1.89%	0.712%
20	11.242	3160	3173	3198	rBV	445041	724450	13.56%	5.112%
21	11.615	3278	3289	3313	rBV	392532	641457	12.01%	4.526%




Sum of corrected areas: 14172388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029201.D
Acq On : 20 Nov 2022 03:47
Operator : SY/MD
Sample : N5651-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

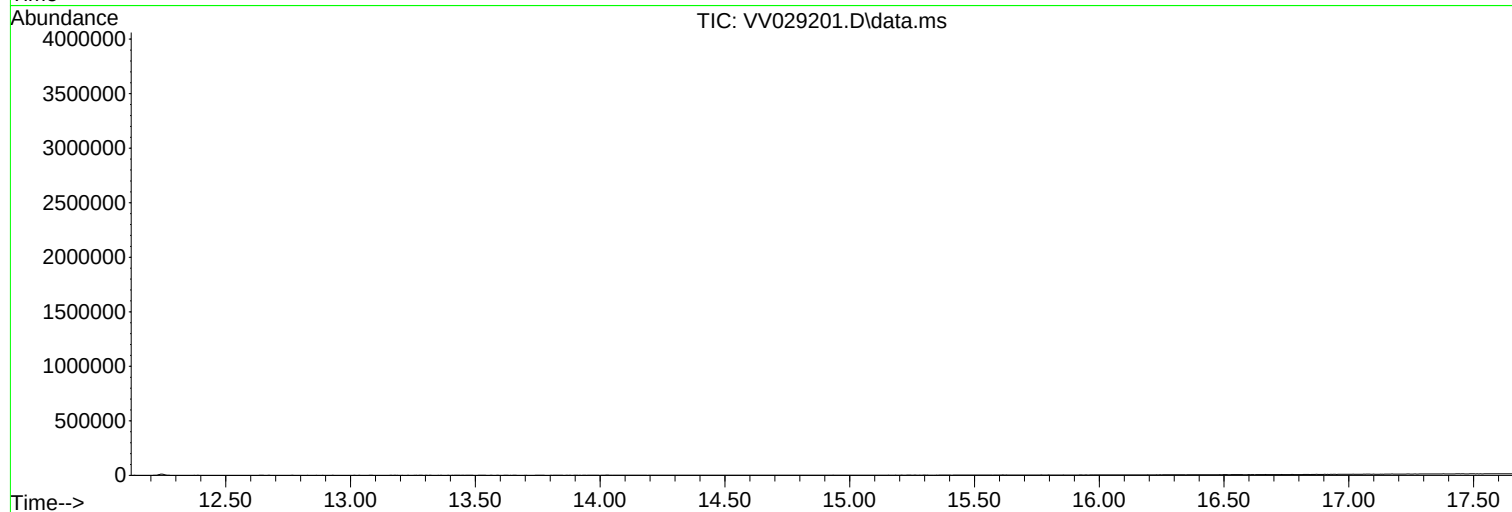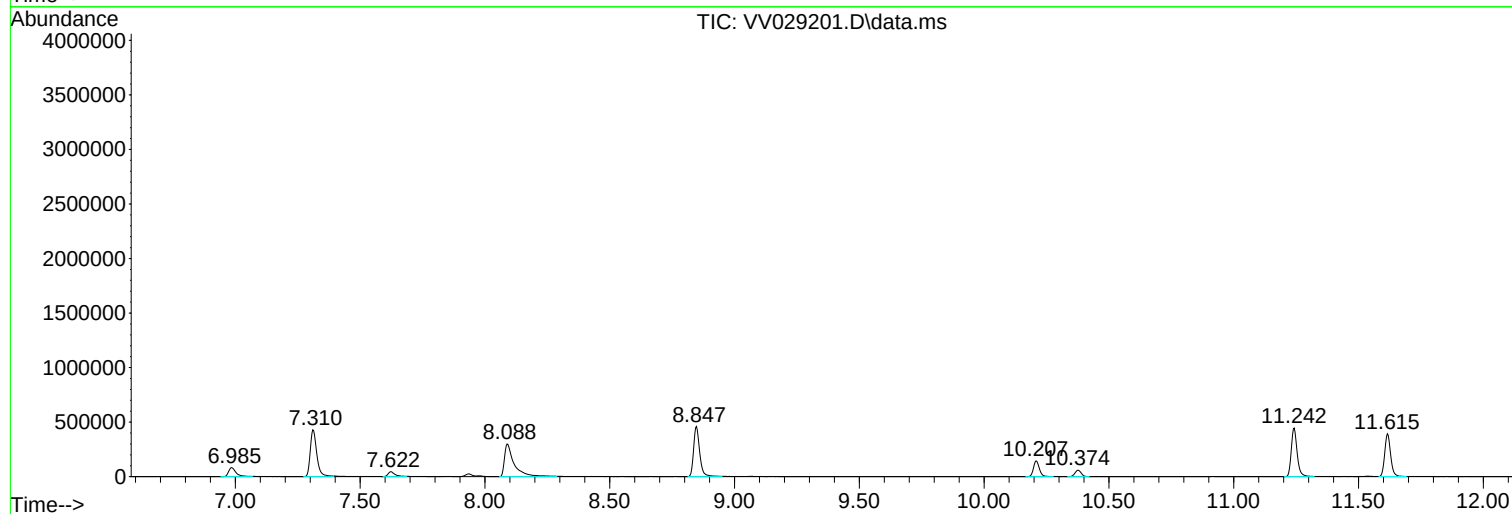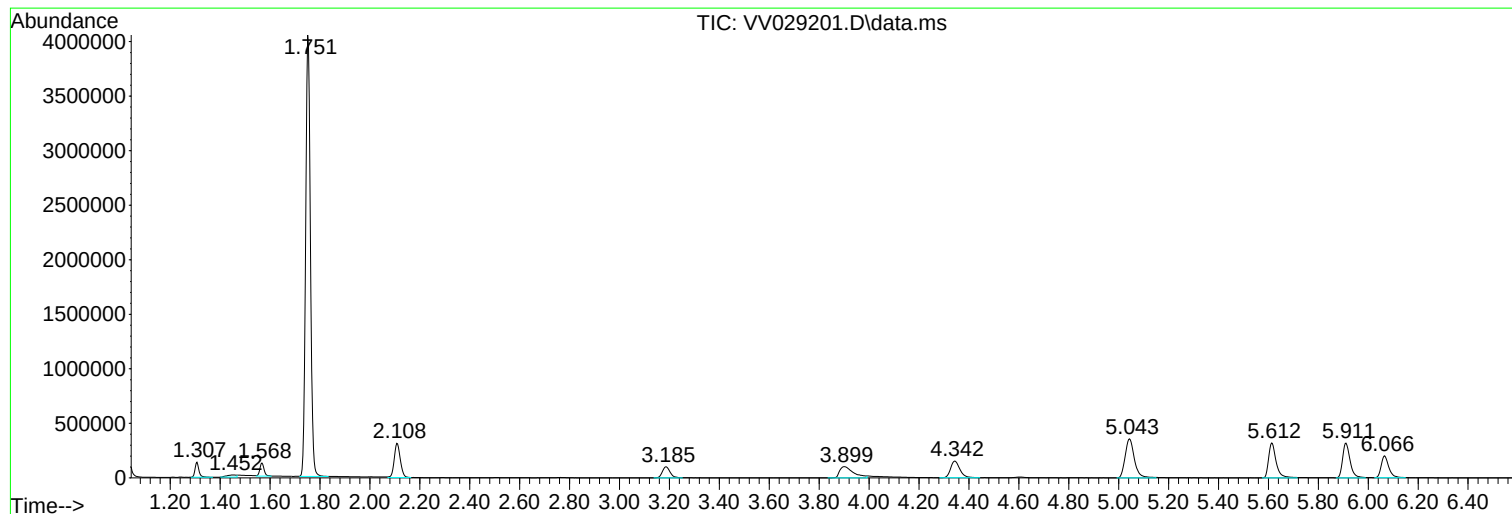

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029201.D
Acq On : 20 Nov 2022 03:47
Operator : SY/MD
Sample : N5651-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111922\
Data File : VV029201.D
Acq On : 20 Nov 2022 03:47
Operator : SY/MD
Sample : N5651-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1G5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc