


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111925\
Data File : VV039403.D
Acq On : 19 Nov 2025 08:56
Operator : SY/MD
Sample : BFB213
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB213

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111925WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 20 03:43:48 2025

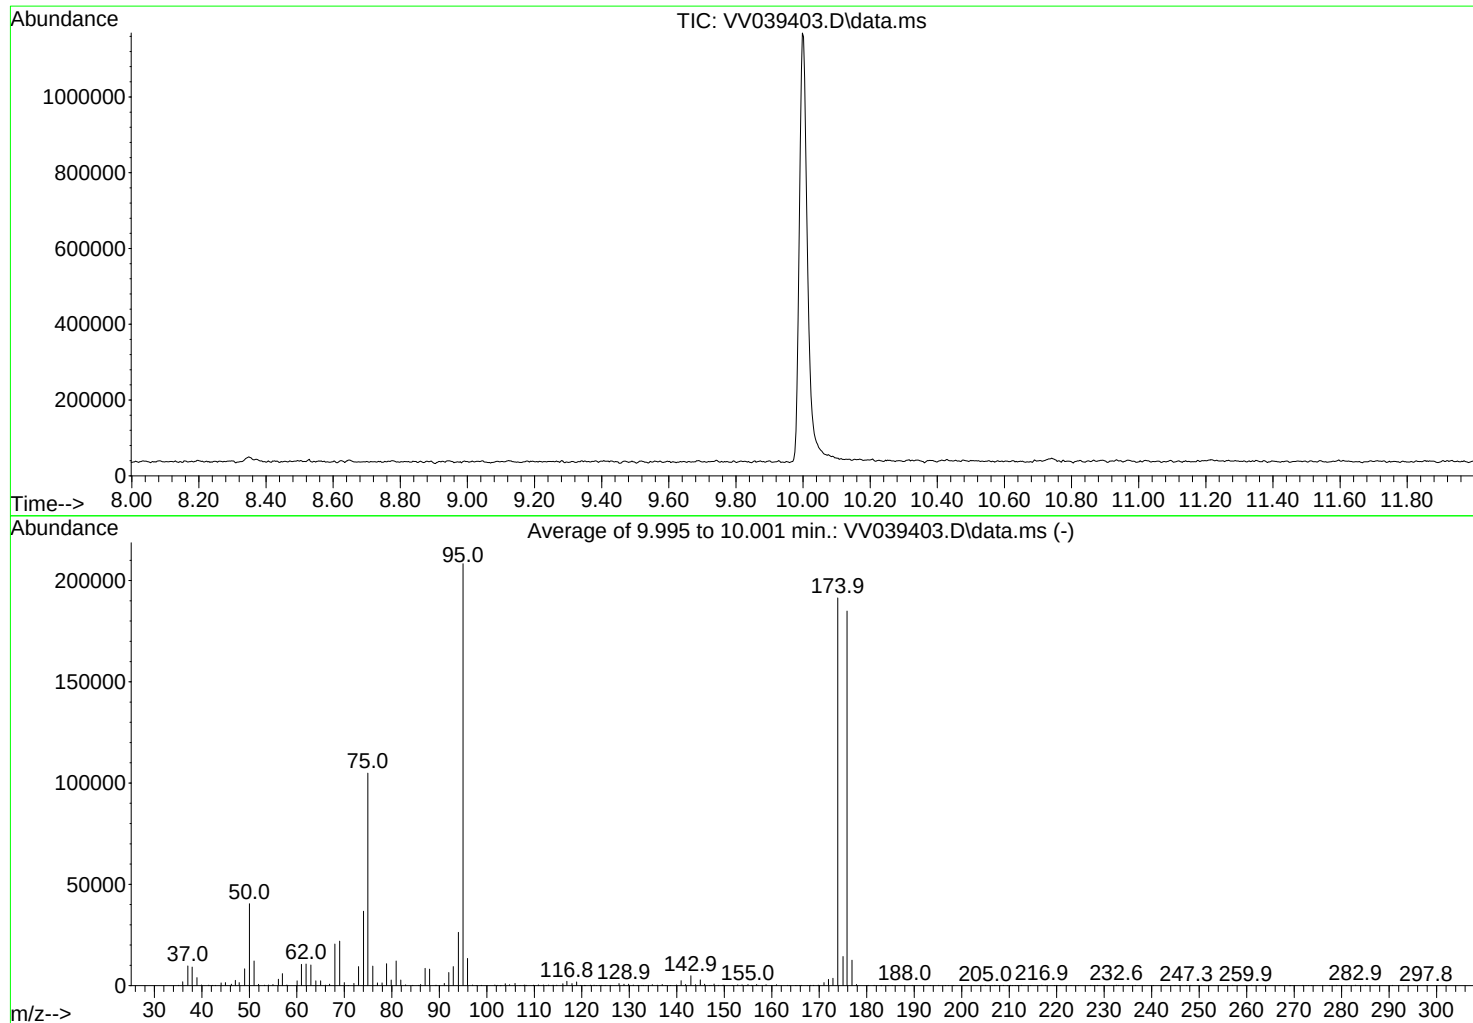

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	40392	PASS
75	95	30	80	50.4	104924	PASS
95	95	100	100	100.0	208298	PASS
96	95	5	9	6.4	13406	PASS
173	174	0.00	2	1.9	3591	PASS
174	95	50	120	91.9	191424	PASS
175	174	5	9	7.5	14342	PASS
176	174	95	105	96.6	184922	PASS
177	176	5	10	6.8	12518	PASS