

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112018\
 Data File : VV008685.D
 Acq On : 20 Nov 2018 19:49
 Operator : SY/MD
 Sample : J5997-05MSD 50X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YA3MSD

Quant Time: Nov 21 01:37:08 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 21 01:28:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	267984	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	246183	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	110320	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77856	41.18	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.36%
7) Chloroethane-d5	1.57	69	37899	36.70	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	73.40%
11) 1,1-Dichloroethene-d2	2.13	63	145707	46.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.40%
21) 2-Butanone-d5	3.94	46	141431	91.78	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.78%
24) Chloroform-d	4.41	84	165462	43.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.42%
26) 1,2-Dichloroethane-d4	5.08	65	113701	46.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.84%
32) Benzene-d6	5.10	84	355793	46.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.92%
36) 1,2-Dichloropropane-d6	6.12	67	113394	47.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.74%
41) Toluene-d8	7.36	98	319167	46.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.88%
43) trans-1,3-Dichloropropene-	7.67	79	42271	39.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.96%
47) 2-Hexanone-d5	8.14	63	97255	89.85	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.85%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	136463	41.80	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	111605	46.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.70%

Target Compounds

					Qvalue
9) Trichlorofluoromethane	2.13	101	1116	0.425 ug/L #	32
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	1116	0.736 ug/L #	17
12) 1,1-Dichloroethene	2.14	96	71001	52.183 ug/L	91
20) cis-1,2-Dichloroethene	3.97	96	6672	3.092 ug/L	76
27) 1,2-Dichloroethane	5.15	62	3759	1.288 ug/L #	74
29) Cyclohexane	4.73	56	6877	2.062 ug/L #	100
33) Benzene	5.15	78	410909	51.918 ug/L	100
34) Trichloroethene	5.96	95	102898	49.057 ug/L	91
35) Methylcyclohexane	6.18	83	48557	14.020 ug/L	96
37) 1,2-Dichloropropane	6.12	63	12047	5.635 ug/L #	94
39) cis-1,3-Dichloropropene	7.04	75	2878	0.947 ug/L #	71
44) trans-1,3-Dichloropropene	7.67	75	1914	0.693 ug/L	89
51) Chlorobenzene	8.93	112	266547	50.901 ug/L	93
52) Ethylbenzene	9.06	91	547949	60.677 ug/L	99
53) m,p-Xylene	9.18	106	637067	191.977 ug/L	91
54) o-xylene	9.59	106	198704	60.217 ug/L	93
55) Styrene	9.59	104	9563	1.738 ug/L #	1


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112018\
Data File : VV008685.D
Acq On : 20 Nov 2018 19:49
Operator : SY/MD
Sample : J5997-05MSD 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YA3MSD

Quant Time: Nov 21 01:37:08 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 21 01:28:05 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
56) Isopropylbenzene	9.98	105	15441	1.780	ug/L	96
69) Naphthalene	13.56	128	5424	0.975	ug/L #	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

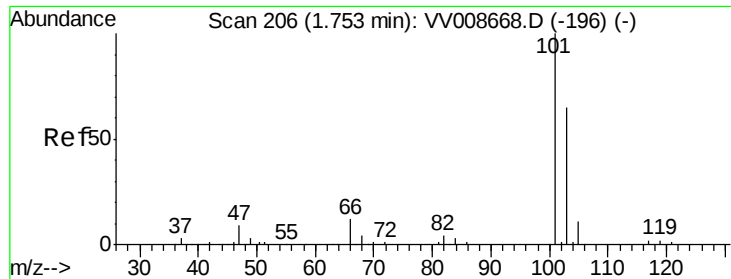

#9

Trichlorofluoromethane

Concen: 0.425 ug/L

RT: 2.13 min Scan# 324

Delta R.T. 0.36 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :





E3YA3MSD

Tgt Ion:101 Resp: 1116

Ion Ratio Lower Upper

101 100

103 9.8 50.2 75.4#

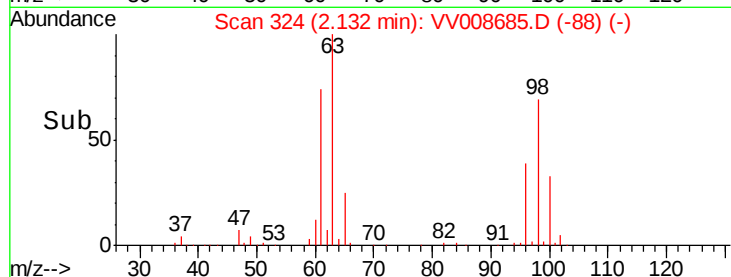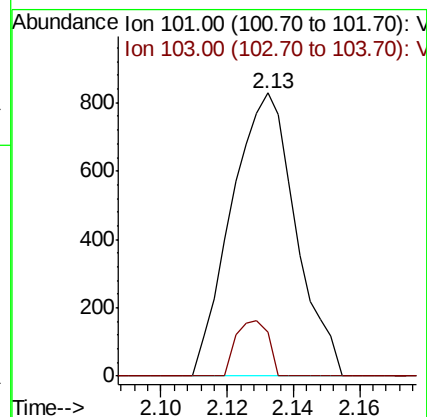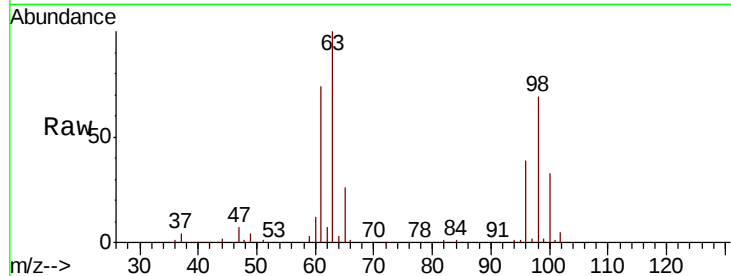

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.736 ug/L

RT: 2.13 min Scan# 324

Delta R.T. -0.01 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49




Tgt Ion:101 Resp: 1116


Ion Ratio Lower Upper

101 100

85 0.0 37.0 55.6#

151 0.0 63.8 95.8#

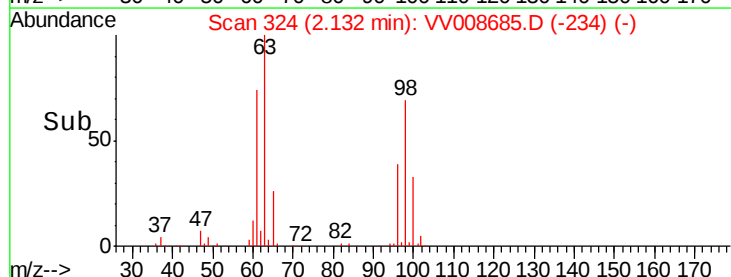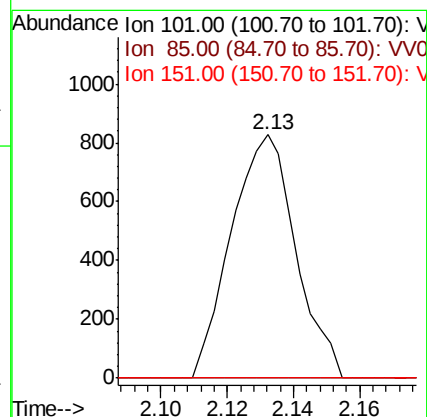

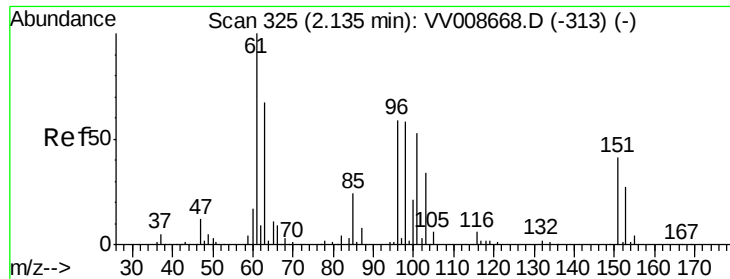

#12

1,1-Dichloroethene

Concen: 52.183 ug/L

RT: 2.14 min Scan# 326

Delta R.T. -0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :

E3YA3MSD





Tgt Ion: 96 Resp: 71001

Ion Ratio Lower Upper

96 100

61 173.6 120.3 223.3

63 137.9 113.3 210.5

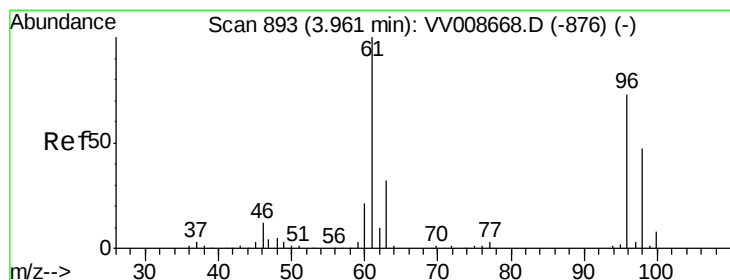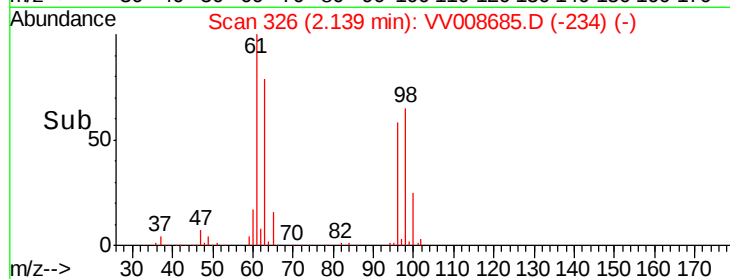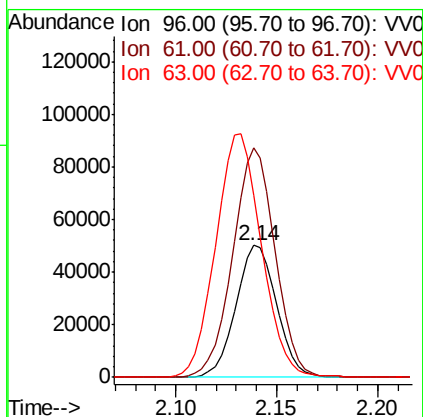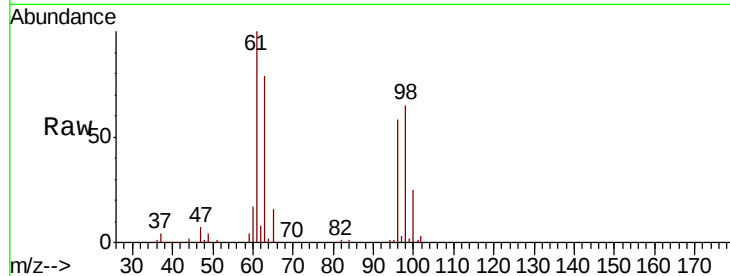

#20

cis-1,2-Dichloroethene

Concen: 3.092 ug/L

RT: 3.97 min Scan# 895

Delta R.T. 0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49




Tgt Ion: 96 Resp: 6672


Ion Ratio Lower Upper

96 100

61 138.1 78.8 146.3

68 0.0 0.0 0.0

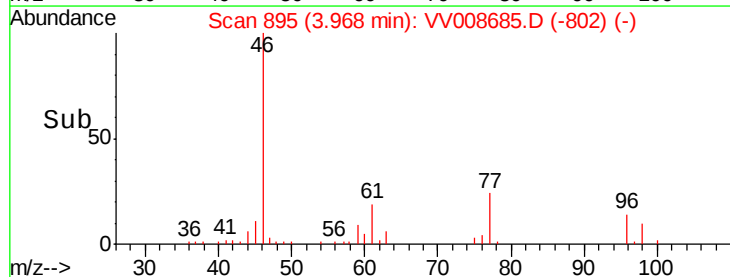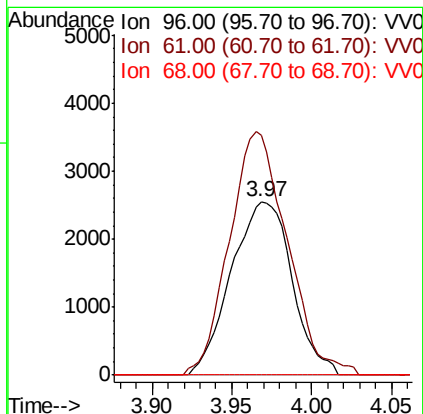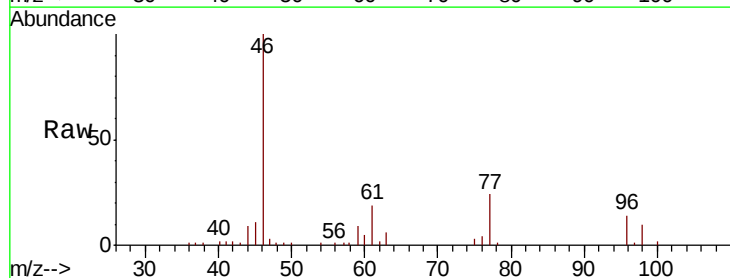

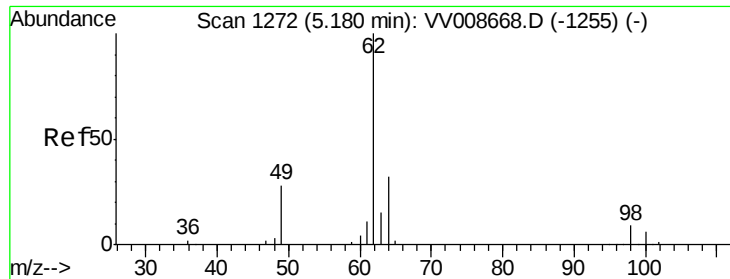

#27

1,2-Dichloroethane

Concen: 1.288 ug/L

RT: 5.15 min Scan# 1263

Delta R.T. -0.03 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :


E3YA3MSD

Tgt Ion: 62 Resp: 3759

Ion Ratio Lower Upper




62 100

98 0.0 7.4 11.2#

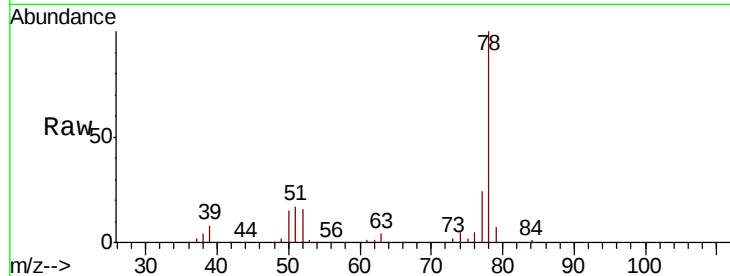

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 98.00 (97.70 to 98.70): VV0

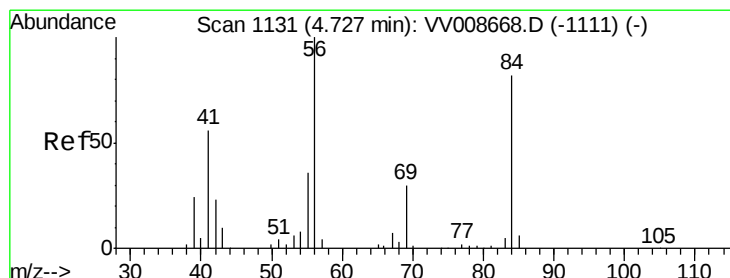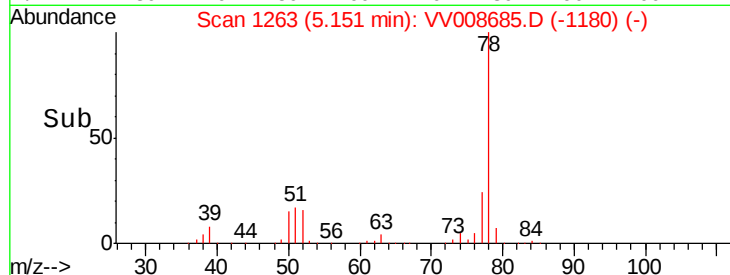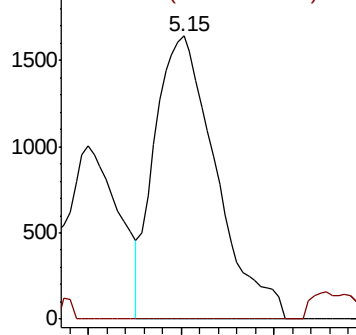

#29

Cyclohexane

Concen: 2.062 ug/L

RT: 4.73 min Scan# 1131

Delta R.T. -0.01 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49


Tgt Ion: 56 Resp: 6877

Ion Ratio Lower Upper

56 100

69 26.1 0.0 0.0#



84 88.1 0.0 0.0#

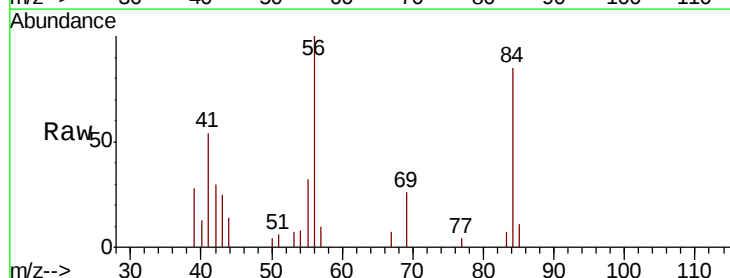


Abundance Ion 56.00 (55.70 to 56.70): VV0

Ion 69.00 (68.70 to 69.70): VV0

Ion 84.00 (83.70 to 84.70): VV0

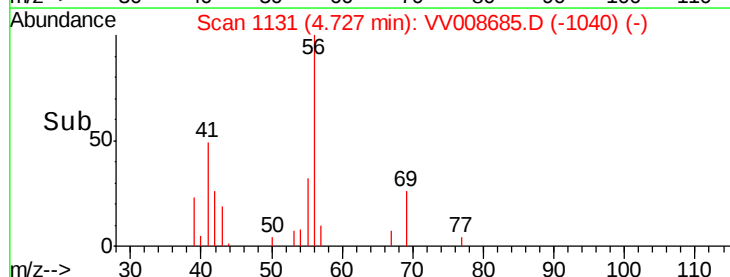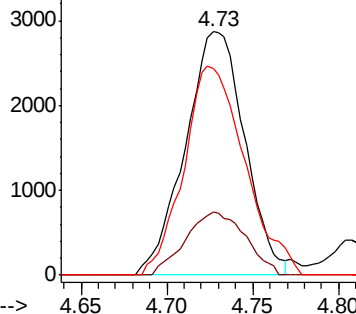

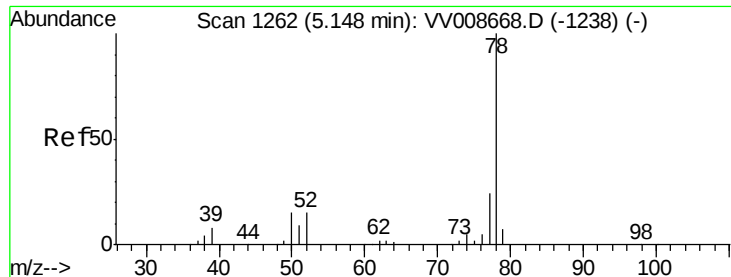

#33

Benzene

Concen: 51.918 ug/L

RT: 5.15 min Scan# 1263





Delta R.T. 0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :
MSVOA_V
ClientSampleId :
E3YA3MSD

Tgt Ion: 78 Resp: 410909

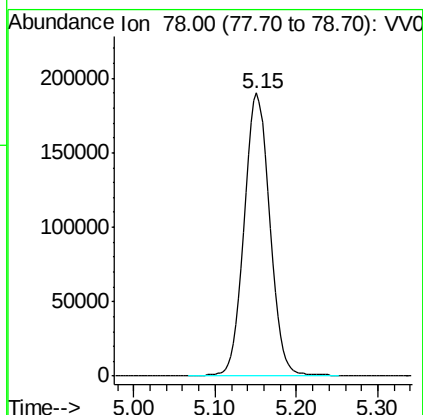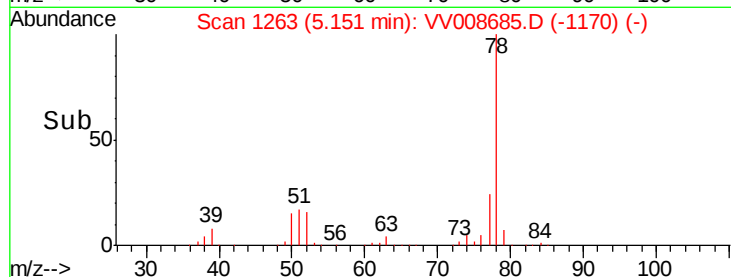

#34

Trichloroethene

Concen: 49.057 ug/L

RT: 5.96 min Scan# 1515

Delta R.T. -0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Tgt Ion: 95 Resp: 102898




Ion	Ratio	Lower	Upper
95	100		
97	63.7	43.8	81.3
132	93.7	58.3	108.3
130	98.4	60.3	112.1


95 100

97 63.7 43.8 81.3

132 93.7 58.3 108.3

130 98.4 60.3 112.1


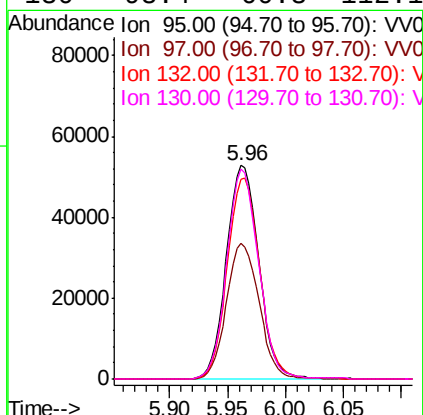
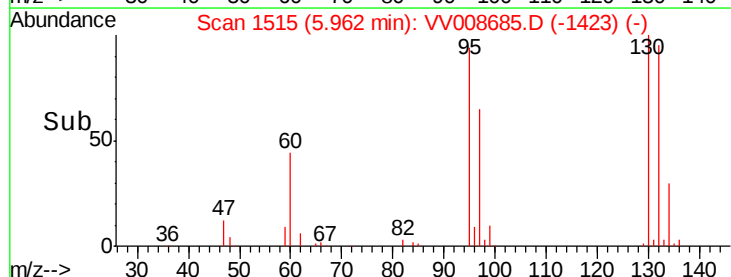



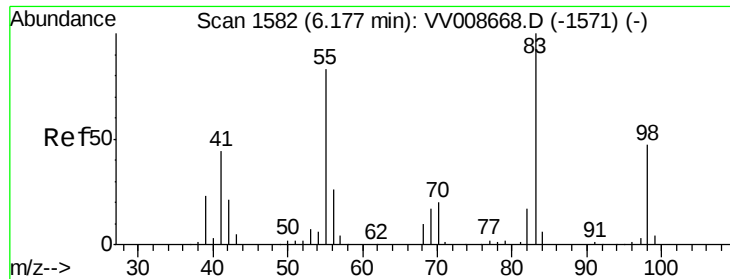

#35
Methylcyclohexane
Concen: 14.020 ug/L
RT: 6.18 min Scan# 1583
Delta R.T. 0.00 min
Lab File: VV008685.D
Acq: 20 Nov 2018 19:49




Instrument :
MSVOA_V
ClientSampleId :
E3YA3MSD


Tgt Ion: 83 Resp: 48557
Ion Ratio Lower Upper
83 100
55 82.3 63.0 94.6
98 46.6 35.4 53.0

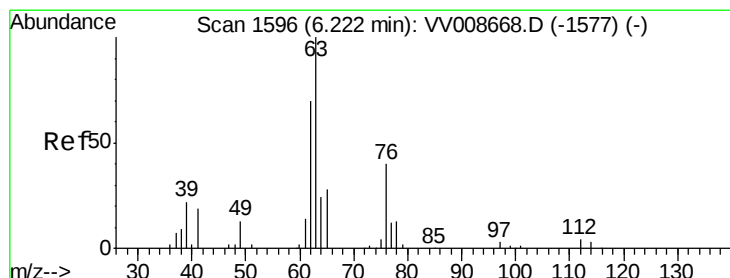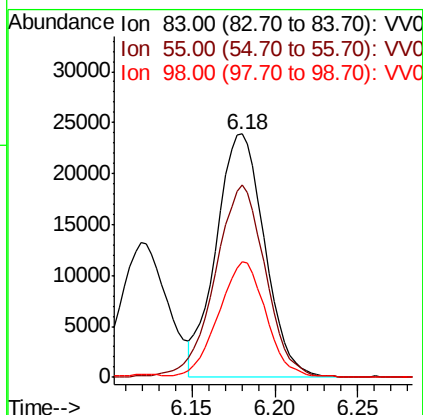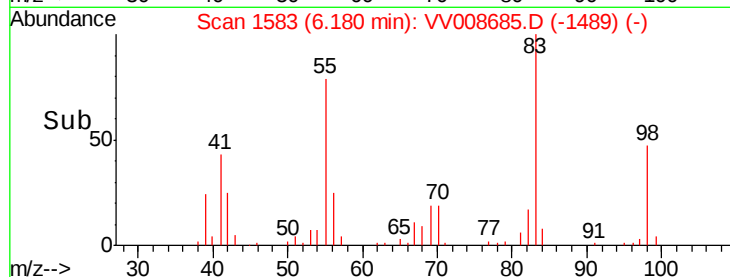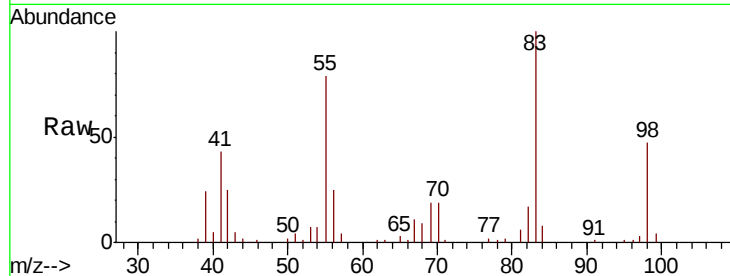

#37
1,2-Dichloropropane
Concen: 5.635 ug/L
RT: 6.12 min Scan# 1564
Delta R.T. -0.10 min
Lab File: VV008685.D
Acq: 20 Nov 2018 19:49

Tgt Ion: 63 Resp: 12047
Ion Ratio Lower Upper
63 100
112 0.0 1.6 2.4#

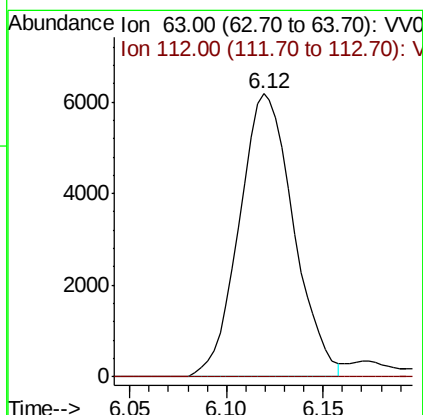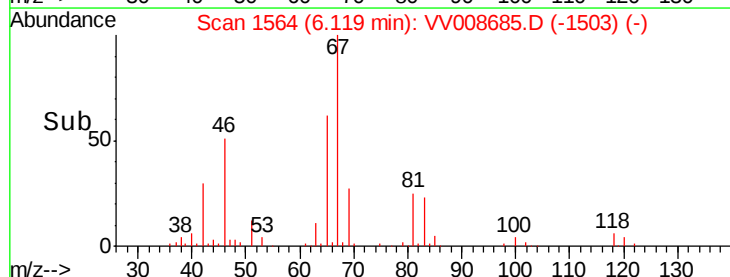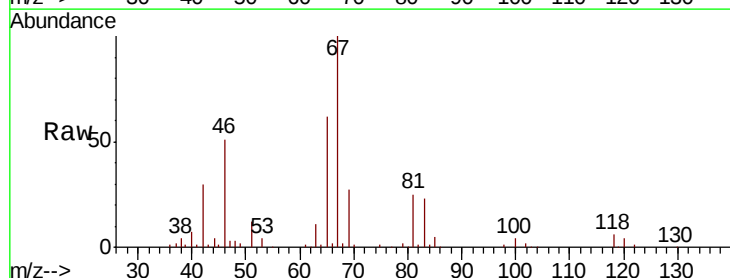

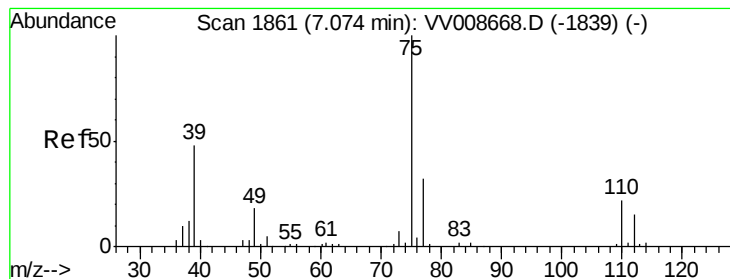

#39

cis-1,3-Dichloropropene

Concen: 0.947 ug/L

RT: 7.04 min Scan# 1849

Delta R.T. -0.04 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :


E3YA3MSD

Tgt Ion: 75 Resp: 2878

Ion Ratio Lower Upper




75 100

77 44.3 20.2 37.4#

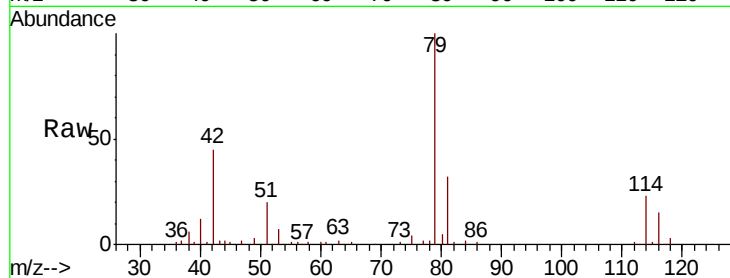

Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 77.00 (76.70 to 77.70): VV0

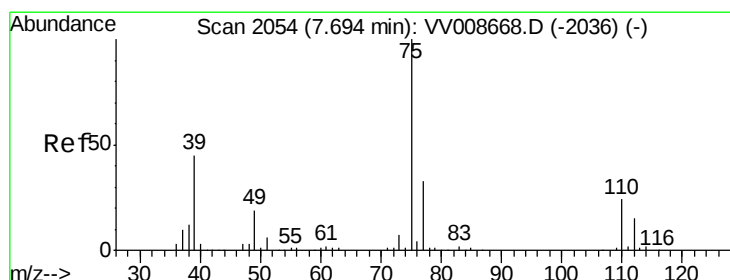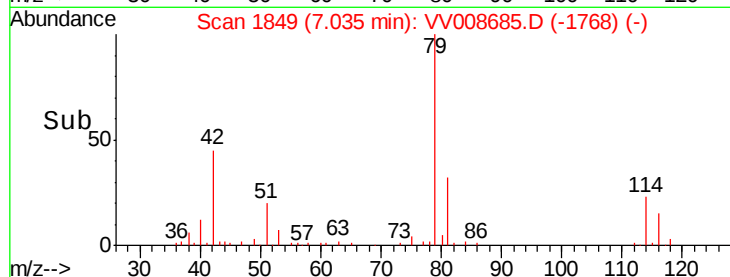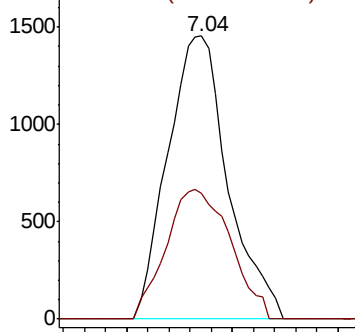

#44

trans-1,3-Dichloropropene

Concen: 0.693 ug/L

RT: 7.67 min Scan# 2045

Delta R.T. -0.03 min

Lab File: VV008685.D


Acq: 20 Nov 2018 19:49

Tgt Ion: 75 Resp: 1914

Ion Ratio Lower Upper



75 100


77 41.5 24.6 45.8

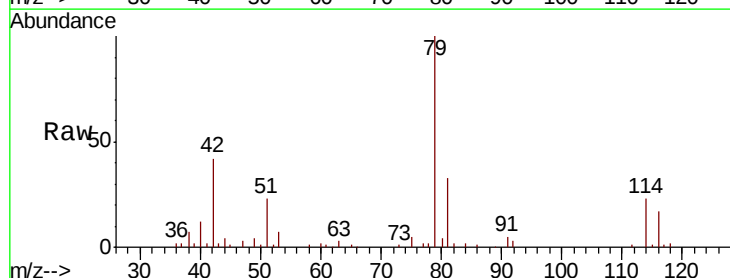

Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 77.00 (76.70 to 77.70): VV0

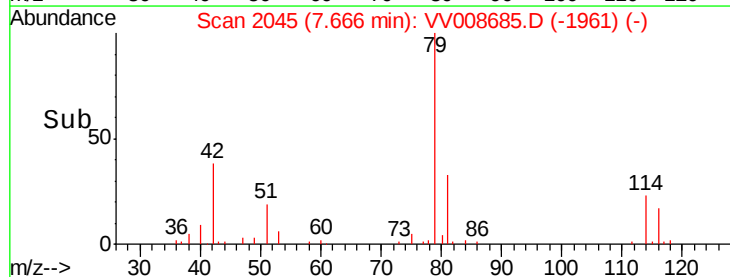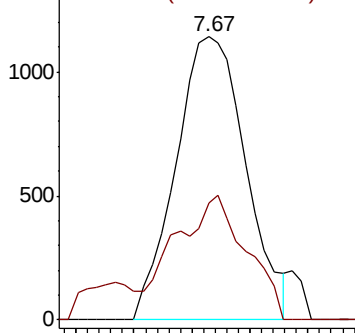

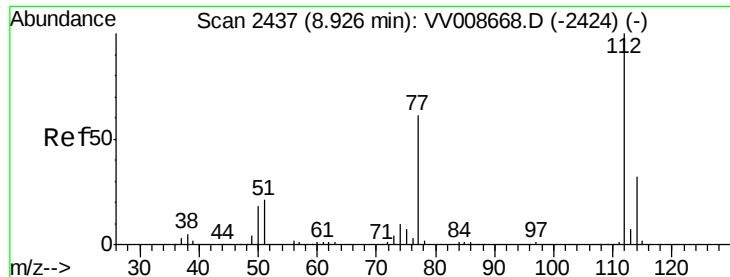

#51

Chlorobenzene

Concen: 50.901 ug/L

RT: 8.93 min Scan# 2437

Delta R.T. 0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :

E3YA3MSD


Tgt Ion: 112 Resp: 266547

Ion Ratio Lower Upper

112 100

114 31.5 22.9 42.5




77 60.1 53.8 80.6

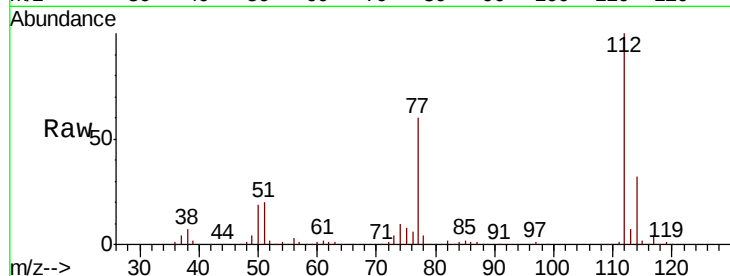

Abundance Ion 112.00 (111.70 to 112.70): V

Ion 114.00 (113.70 to 114.70): V

Ion 77.00 (76.70 to 77.70): V

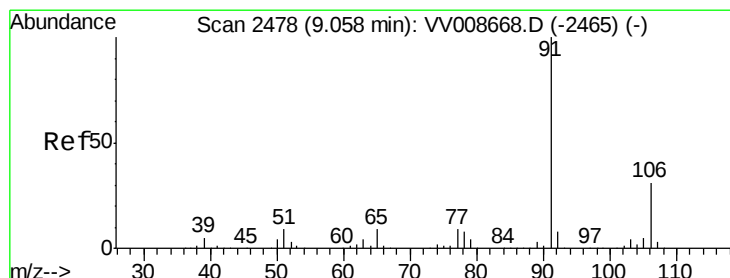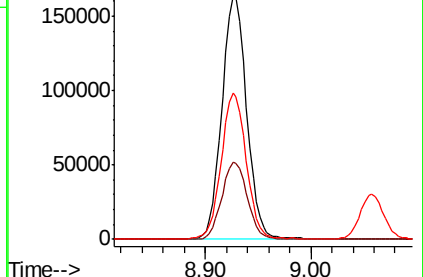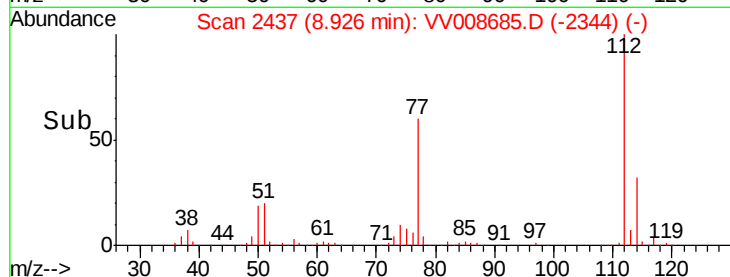

#52

Ethylbenzene

Concen: 60.677 ug/L

RT: 9.06 min Scan# 2478

Delta R.T. 0.00 min

Lab File: VV008685.D


Acq: 20 Nov 2018 19:49

Tgt Ion: 91 Resp: 547949

Ion Ratio Lower Upper



91 100


106 30.9 21.2 39.4

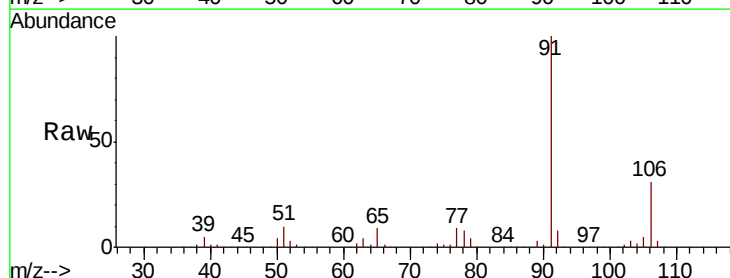

Abundance Ion 91.00 (90.70 to 91.70): V

Ion 106.00 (105.70 to 106.70): V

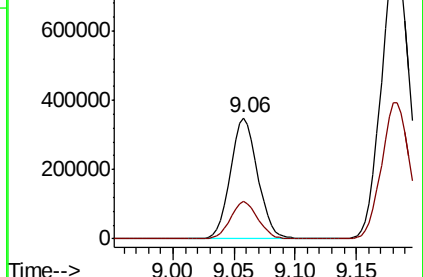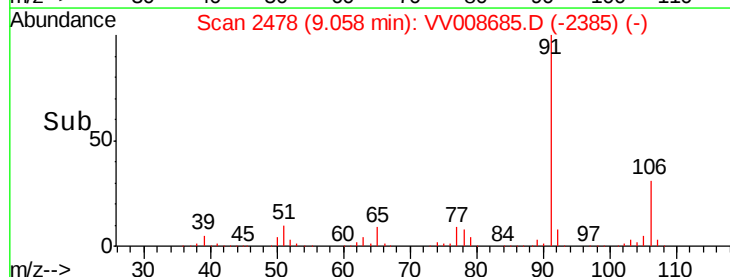

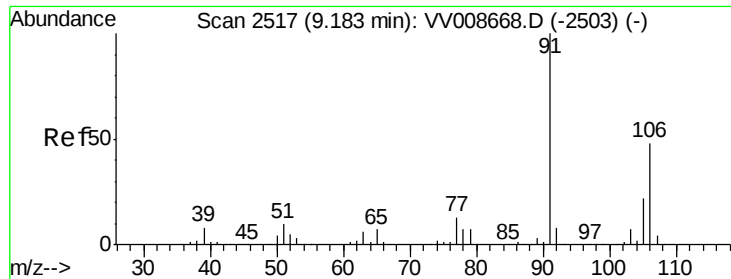

#53

m,p-Xylene

Concen: 191.977 ug/L

RT: 9.18 min Scan# 2517

Delta R.T. 0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :


E3YA3MSD

Tgt Ion:106 Resp: 637067

Ion Ratio Lower Upper




106 100

91 207.0 154.7 287.3

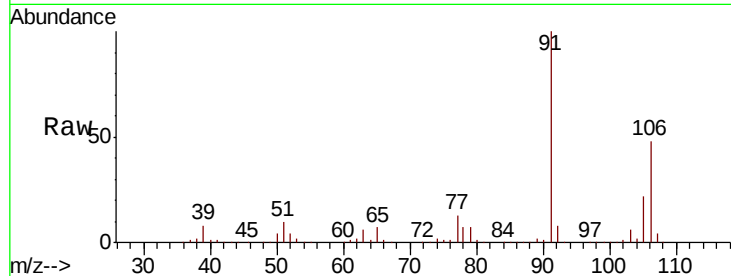

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VV0

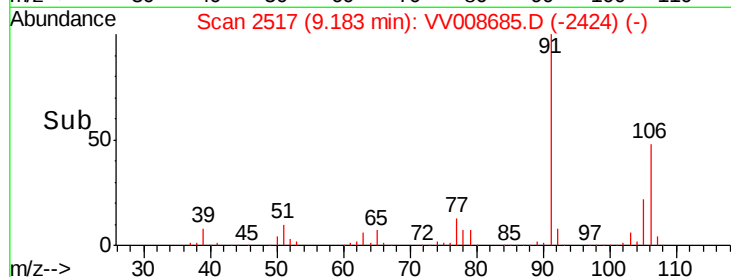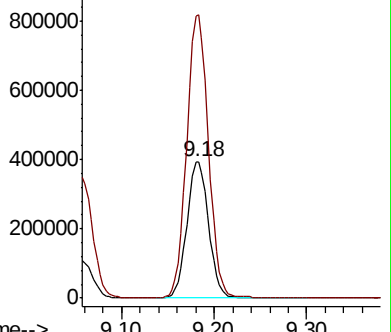

#54

o-xylene

Concen: 60.217 ug/L

RT: 9.59 min Scan# 2643

Delta R.T. 0.00 min

Lab File: VV008685.D


Acq: 20 Nov 2018 19:49

Tgt Ion:106 Resp: 198704

Ion Ratio Lower Upper



106 100


91 220.5 146.7 272.5



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VV0

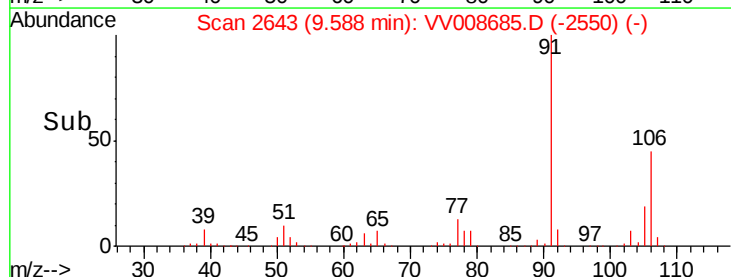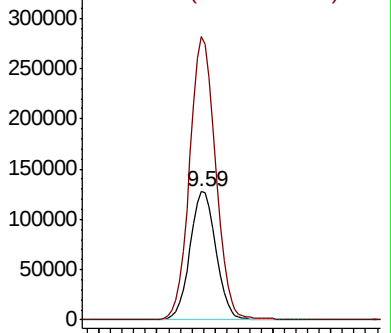

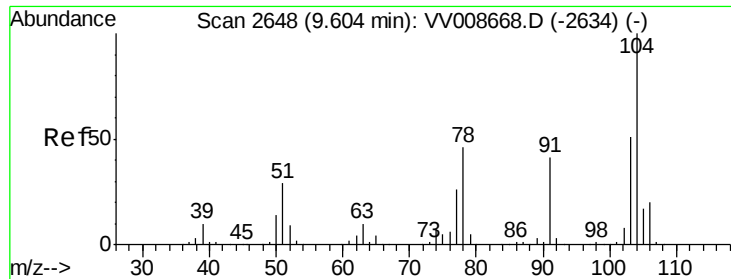

#55

Styrene

Concen: 1.738 ug/L

RT: 9.59 min Scan# 2643

Delta R.T. -0.02 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :


E3YA3MSD

Tgt Ion:104 Resp: 9563

Ion Ratio Lower Upper




104 100

78 324.9 32.7 60.7#



Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VV0

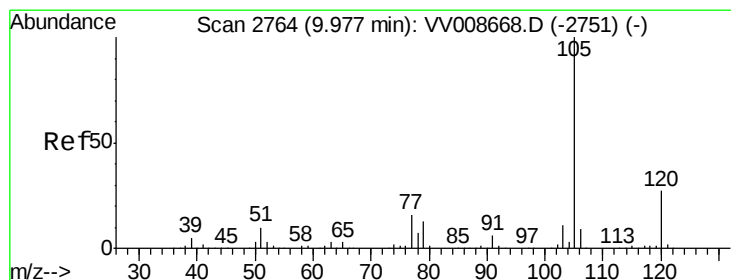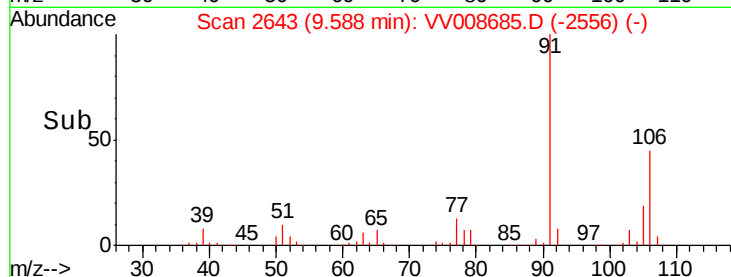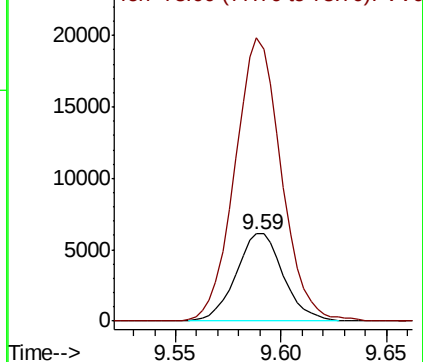

#56

Isopropylbenzene

Concen: 1.780 ug/L

RT: 9.98 min Scan# 2764

Delta R.T. 0.00 min

Lab File: VV008685.D

Acq: 20 Nov 2018 19:49


Tgt Ion:105 Resp: 15441

Ion Ratio Lower Upper

105 100

120 28.9 20.5 30.7



77 15.9 12.8 19.2




Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VV0

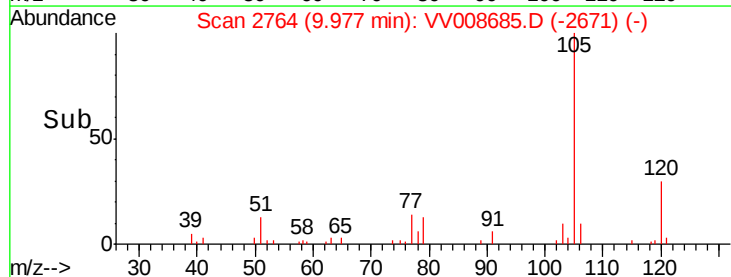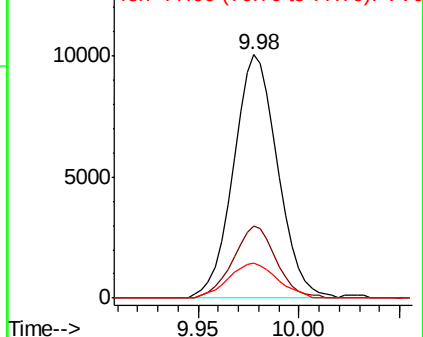

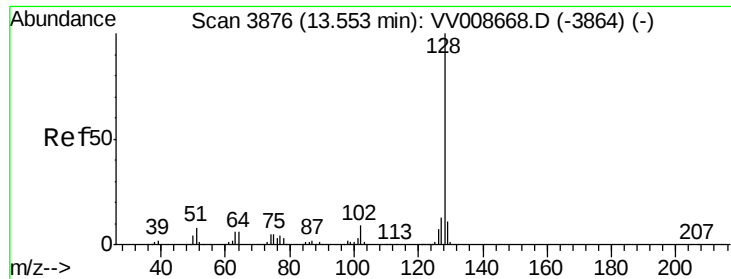

#69

Naphthalene

Concen: 0.975 ug/L

RT: 13.56 min Scan# 3877

Delta R.T. 0.00 min

Lab File: VV008685.D


Acq: 20 Nov 2018 19:49

Instrument :

MSVOA_V

ClientSampleId :

E3YA3MSD



Tgt Ion:	128	Resp:	5424
Ion	Ratio	Lower	Upper
128	100		
127	5.3	9.4	14.0#
129	8.2	8.9	13.3#

