


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112018\
 Data File : VV008664.D
 Acq On : 20 Nov 2018 09:39
 Operator : SY/MD
 Sample : BFB47
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111518WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 16 23:18:19 2018

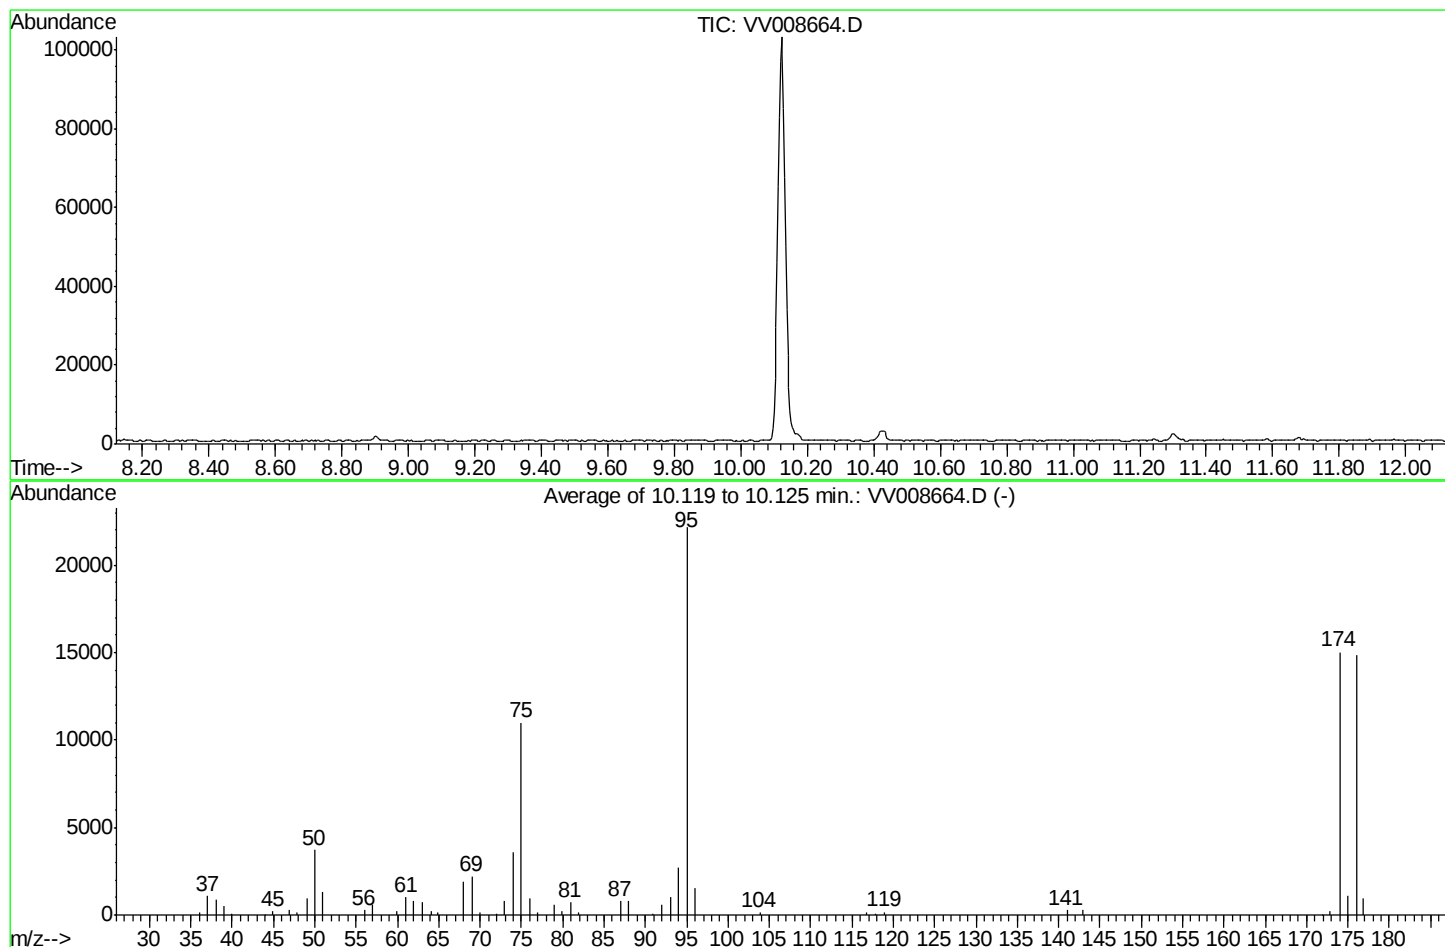

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	3719	PASS
75	95	30	80	49.6	10996	PASS
95	95	100	100	100.0	22157	PASS
96	95	5	9	7.0	1551	PASS
173	174	0.00	2	1.5	228	PASS
174	95	50	120	67.8	15021	PASS
175	174	5	9	7.5	1130	PASS
176	174	95	101	99.0	14876	PASS
177	176	5	9	6.6	980	PASS

m/z	Abundance
36.00	168.0
37.00	1041.0
38.00	814.0
39.00	465.0
39.90	351.0
44.00	622.0
44.90	209.0
46.90	292.0
47.90	121.0
49.00	1030.0
50.00	3689.0
51.00	1203.0
56.00	257.0
57.00	602.0
59.90	158.0
61.00	995.0
62.00	823.0
62.90	702.0
64.10	193.0
64.80	125.0
68.00	1867.0
69.00	2245.0
70.00	164.0
72.90	801.0
74.00	3652.0
75.00	10537.0
76.00	940.0
76.90	131.0
78.90	516.0
79.90	207.0
80.90	662.0
81.90	153.0
87.00	849.0
88.00	794.0
92.00	677.0
93.00	1012.0
94.00	2778.0
95.00	22088.0
96.00	1519.0
103.90	107.0
116.80	116.0
117.90	122.0
118.90	180.0
141.00	229.0
142.90	265.0
172.80	195.0
174.00	14387.0
175.00	1180.0
176.00	14119.0
176.90	813.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

Scan 2798 (10.087 min): VV008664.D
BFB47

m/z	Abundance
39.90	322.0
44.00	636.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
36.00	203.0
37.00	1057.0
38.00	900.0
39.10	522.0
39.90	408.0
44.00	688.0
44.90	172.0
46.90	233.0
47.80	144.0
49.00	818.0
50.00	3674.0
51.00	1351.0
56.00	312.0
57.00	513.0
59.90	287.0
61.00	961.0
62.00	763.0
63.00	811.0
64.10	164.0
64.90	126.0
68.00	1862.0
69.00	2030.0
70.10	147.0
72.00	160.0
73.00	812.0
74.00	3374.0
75.00	11111.0
76.10	983.0
77.00	170.0
78.90	623.0
80.00	229.0
80.90	684.0
82.00	138.0
87.00	705.0
87.90	761.0
90.90	131.0
92.00	552.0
93.00	941.0
94.00	2471.0
95.00	21472.0
96.00	1517.0
103.80	118.0
116.80	132.0
119.00	147.0
141.00	289.0
142.90	246.0
171.80	101.0
172.80	256.0
174.00	15179.0
175.00	1035.0
176.00	15050.0
176.90	1101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
36.00	178.0
37.00	1118.0
38.00	910.0
39.00	531.0
39.90	390.0
44.00	644.0
44.90	208.0
46.90	273.0
47.90	152.0
49.00	985.0
50.00	3795.0
50.90	1351.0
56.00	301.0
57.00	596.0
59.90	230.0
61.00	1074.0
62.00	797.0
63.00	780.0
64.10	225.0
64.90	122.0
68.00	1949.0
69.00	2214.0
70.00	157.0
72.00	150.0
72.90	851.0
74.00	3766.0
75.00	11342.0
76.10	1020.0
77.00	176.0
78.90	576.0
79.90	239.0
80.90	749.0
81.90	159.0
87.00	847.0
87.90	820.0
90.90	107.0
92.00	623.0
93.00	1043.0
94.00	2819.0
95.00	22912.0
96.00	1618.0
103.80	122.0
116.80	125.0
117.80	111.0
118.90	187.0
141.00	291.0
142.90	279.0
172.80	234.0
174.00	15497.0
175.00	1176.0
176.00	15460.0
176.90	1027.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47