


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112019\
 Data File : VV013684.D
 Acq On : 20 Nov 2019 09:25
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Nov 22 03:55:18 2019

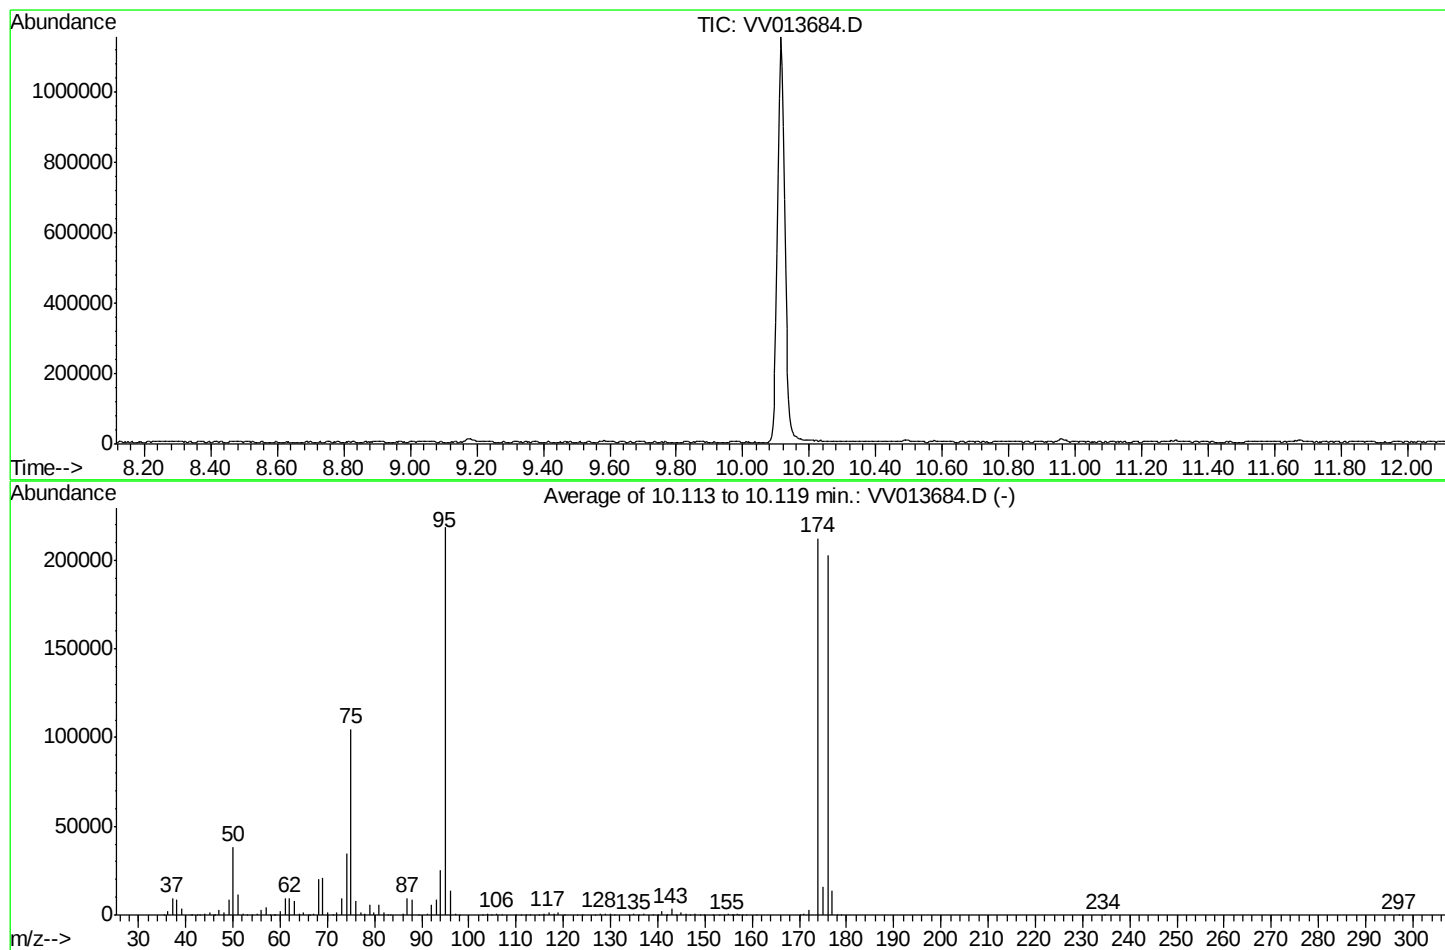

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	38290	PASS
75	95	30	80	48.0	104913	PASS
95	95	100	100	100.0	218453	PASS
96	95	5	9	6.4	14077	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.1	212160	PASS
175	174	5	9	7.4	15607	PASS
176	174	95	101	95.5	202517	PASS
177	176	5	9	6.8	13675	PASS

m/z	Abundance
35.40	198.0
36.10	1913.0
37.10	10063.0
38.00	8589.0
39.10	4037.0
39.90	930.0
41.10	189.0
42.50	101.0
43.10	174.0
44.00	1675.0
45.10	1640.0
46.20	315.0
47.00	2802.0
48.00	1429.0
49.00	8980.0
50.00	39640.0
51.00	11315.0
52.10	533.0
53.00	297.0
54.10	267.0
55.10	585.0
56.00	2525.0
57.10	4667.0
58.00	418.0
58.60	163.0
58.90	108.0
60.00	2171.0
61.00	10049.0
62.00	9659.0
63.00	8400.0
64.10	1335.0
65.00	1697.0
66.20	326.0
67.00	695.0
68.00	21112.0
69.00	21344.0
70.10	1432.0
72.00	1331.0
73.00	9674.0
74.00	35224.0
75.00	107496.0
76.10	8449.0
77.00	1521.0
78.00	824.0
79.00	6167.0
79.90	1837.0
80.90	5714.0
82.00	1298.0
82.90	131.0
83.30	180.0
86.00	535.0
87.00	9545.0
87.90	8749.0
89.40	150.0
91.20	713.0
92.10	5892.0
93.00	8902.0
94.00	24840.0
95.00	221760.0
96.10	14701.0
97.00	485.0
103.00	133.0
103.90	970.0
104.80	331.0
105.90	872.0
106.90	302.0
110.00	223.0
111.00	165.0
112.00	104.0
112.80	232.0
114.80	346.0
115.90	674.0
116.90	1793.0
118.00	840.0
118.90	1312.0
120.30	117.0
122.90	115.0
123.90	194.0
126.70	222.0
127.80	971.0
128.80	484.0
129.90	735.0
130.80	272.0
134.90	503.0
136.90	579.0
139.90	233.0
141.00	2430.0
141.90	283.0
143.00	3622.0
143.80	382.0
145.00	1449.0
145.80	499.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

146.70	201.0
148.00	631.0
148.90	223.0
149.80	179.0
151.90	203.0
153.00	222.0
154.10	110.0
154.90	711.0
155.90	180.0
156.90	375.0
157.10	379.0
158.00	114.0
158.90	322.0
161.00	310.0
170.80	798.0
172.00	3012.0
174.00	208896.0
175.00	15742.0
176.00	199616.0
177.00	13631.0
177.90	337.0
178.80	107.0
297.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.30	171.0
36.10	2066.0
37.10	9940.0
38.10	9127.0
39.10	4166.0
39.90	812.0
41.00	160.0
43.00	181.0
44.00	1695.0
45.10	1676.0
45.80	325.0
46.30	302.0
47.10	2746.0
48.00	1347.0
49.00	9161.0
50.10	39704.0
51.10	11931.0
52.10	618.0
52.90	284.0
54.10	241.0
55.10	707.0
56.00	2625.0
57.10	4665.0
58.00	416.0
58.50	195.0
60.00	2347.0
61.00	9938.0
62.00	10190.0
63.00	8265.0
64.20	1141.0
65.00	1691.0
66.20	221.0
67.00	756.0
68.00	20880.0
69.00	21536.0
70.10	1441.0
71.30	148.0
72.00	1446.0
73.00	9588.0
74.10	36360.0
75.10	108776.0
76.00	8349.0
77.00	1672.0
78.00	842.0
78.90	5904.0
79.90	1857.0
80.90	5881.0
82.00	1373.0
82.90	184.0
86.00	463.0
87.00	9660.0
87.90	9095.0
89.40	152.0
91.20	773.0
92.10	5866.0
93.00	9230.0
94.00	26064.0
95.00	226432.0
96.00	14369.0
97.10	486.0
103.00	192.0
103.90	908.0
104.80	365.0
105.90	974.0
106.90	289.0
110.00	233.0
110.90	216.0
112.00	122.0
112.80	231.0
114.80	333.0
115.90	663.0
116.90	1783.0
117.90	847.0
118.90	1390.0
122.90	121.0
123.90	272.0
126.70	176.0
127.80	973.0
128.80	512.0
129.90	808.0
130.80	251.0
133.80	108.0
134.90	526.0
136.00	134.0
136.90	479.0
138.90	118.0
139.90	257.0
140.90	2271.0
142.10	262.0
143.00	3668.0
143.90	308.0
145.00	1529.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

145.80	397.0
146.70	172.0
148.00	707.0
149.00	276.0
149.80	169.0
151.80	206.0
153.00	275.0
154.10	134.0
154.90	713.0
156.10	144.0
156.90	447.0
157.90	102.0
158.90	279.0
161.00	355.0
170.80	783.0
171.90	3003.0
174.00	219072.0
175.00	15899.0
176.00	209856.0
177.00	14283.0
178.00	310.0
178.80	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.20	162.0
36.10	1921.0
37.10	8792.0
38.00	8886.0
39.10	3606.0
39.90	750.0
41.40	237.0
42.20	151.0
42.90	204.0
44.00	1603.0
45.10	1697.0
45.80	366.0
47.10	2652.0
47.90	1228.0
49.10	8175.0
50.10	35528.0
51.10	11173.0
52.10	648.0
52.80	272.0
54.10	188.0
55.00	653.0
56.10	2528.0
57.10	4401.0
57.90	299.0
60.00	2203.0
61.00	8724.0
62.00	9423.0
63.00	7503.0
64.00	945.0
65.00	1580.0
65.90	201.0
67.00	773.0
68.10	18520.0
69.00	19296.0
70.10	1421.0
71.20	169.0
72.00	1228.0
73.00	8531.0
74.00	33264.0
75.10	98856.0
76.00	7828.0
77.00	1551.0
78.00	780.0
78.90	5263.0
79.90	1759.0
80.90	5786.0
81.90	1335.0
82.90	173.0
86.00	400.0
86.90	9019.0
88.00	8722.0
89.30	118.0
91.10	671.0
92.00	5486.0
93.00	8579.0
94.00	24168.0
95.00	207168.0
96.00	13161.0
97.10	394.0
97.90	131.0
102.90	205.0
103.90	802.0
104.70	408.0
105.90	903.0
106.90	222.0
109.90	230.0
111.00	213.0
112.00	106.0
112.90	209.0
114.80	265.0
115.90	628.0
116.90	1530.0
117.90	841.0
118.90	1286.0
123.90	274.0
126.60	115.0
127.80	843.0
128.80	457.0
129.90	843.0
130.80	244.0
133.70	112.0
134.90	534.0
136.00	175.0
136.90	304.0
138.80	152.0
139.90	202.0
140.90	1956.0
142.00	285.0
143.00	3202.0
143.90	274.0
145.00	1519.0
145.90	332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

146.80	132.0
147.90	649.0
149.00	346.0
149.90	163.0
151.70	179.0
153.00	263.0
154.00	136.0
154.90	642.0
155.70	118.0
156.20	138.0
156.90	497.0
157.80	138.0
158.80	276.0
161.00	364.0
170.00	109.0
170.90	642.0
171.90	2851.0
174.00	208512.0
175.00	15180.0
176.00	198080.0
177.00	13112.0
178.00	241.0
206.90	140.0
234.60	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.70	243.0
36.70	137.0
37.20	164.0
37.90	154.0
39.90	866.0
42.20	168.0
44.00	664.0
45.00	117.0
46.40	182.0
47.20	136.0
51.70	131.0
54.80	109.0
62.70	119.0
64.10	134.0
65.10	131.0
67.60	104.0
71.00	104.0
75.00	129.0
75.70	137.0
78.40	129.0
88.50	173.0
103.00	116.0
113.90	114.0
173.00	102.0
207.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35