

Data File : VV019409.D
Acq On : 20 Nov 2020 09:11
Operator : SY/MD
Sample : VSTDCCC0.5
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB303

Quant Time: Nov 20 23:14:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 20 00:26:09 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	5147	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.88	117	4778	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.28	152	2499	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	3698	0.50	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.00%
4) 1,2-Dichloroethane-d4	5.07	65	2216	0.51	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.00%
7) 1,2-Dichloropropane-d6	6.09	67	2114	0.53	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.00%
8) Toluene-d8	7.33	98	5573	0.48	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.00%
10) 1,1,2,2-Tetrachloroethane-	10.23	84	1113	0.52	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.00%

Target Compounds


						Qvalue
3) Vinyl chloride	1.32	62	3224	0.484	ug/L	99
6) Trichloroethene	5.93	95	1980	0.498	ug/L	100
9) 1,2-Dibromoethane	8.38	107	1111	0.490	ug/L	99
12) 1,2,3-Trichloropropane	10.28	75	936	0.510	ug/L	98
13) 1,2-Dibromo-3-chloropropan	12.44	75	160	0.539	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV019409.D
Acq On : 20 Nov 2020 09:11
Operator : SY/MD
Sample : VSTDCCC0.5
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB303

Quant Time: Nov 20 23:14:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 20 00:26:09 2020
Response via : Initial Calibration

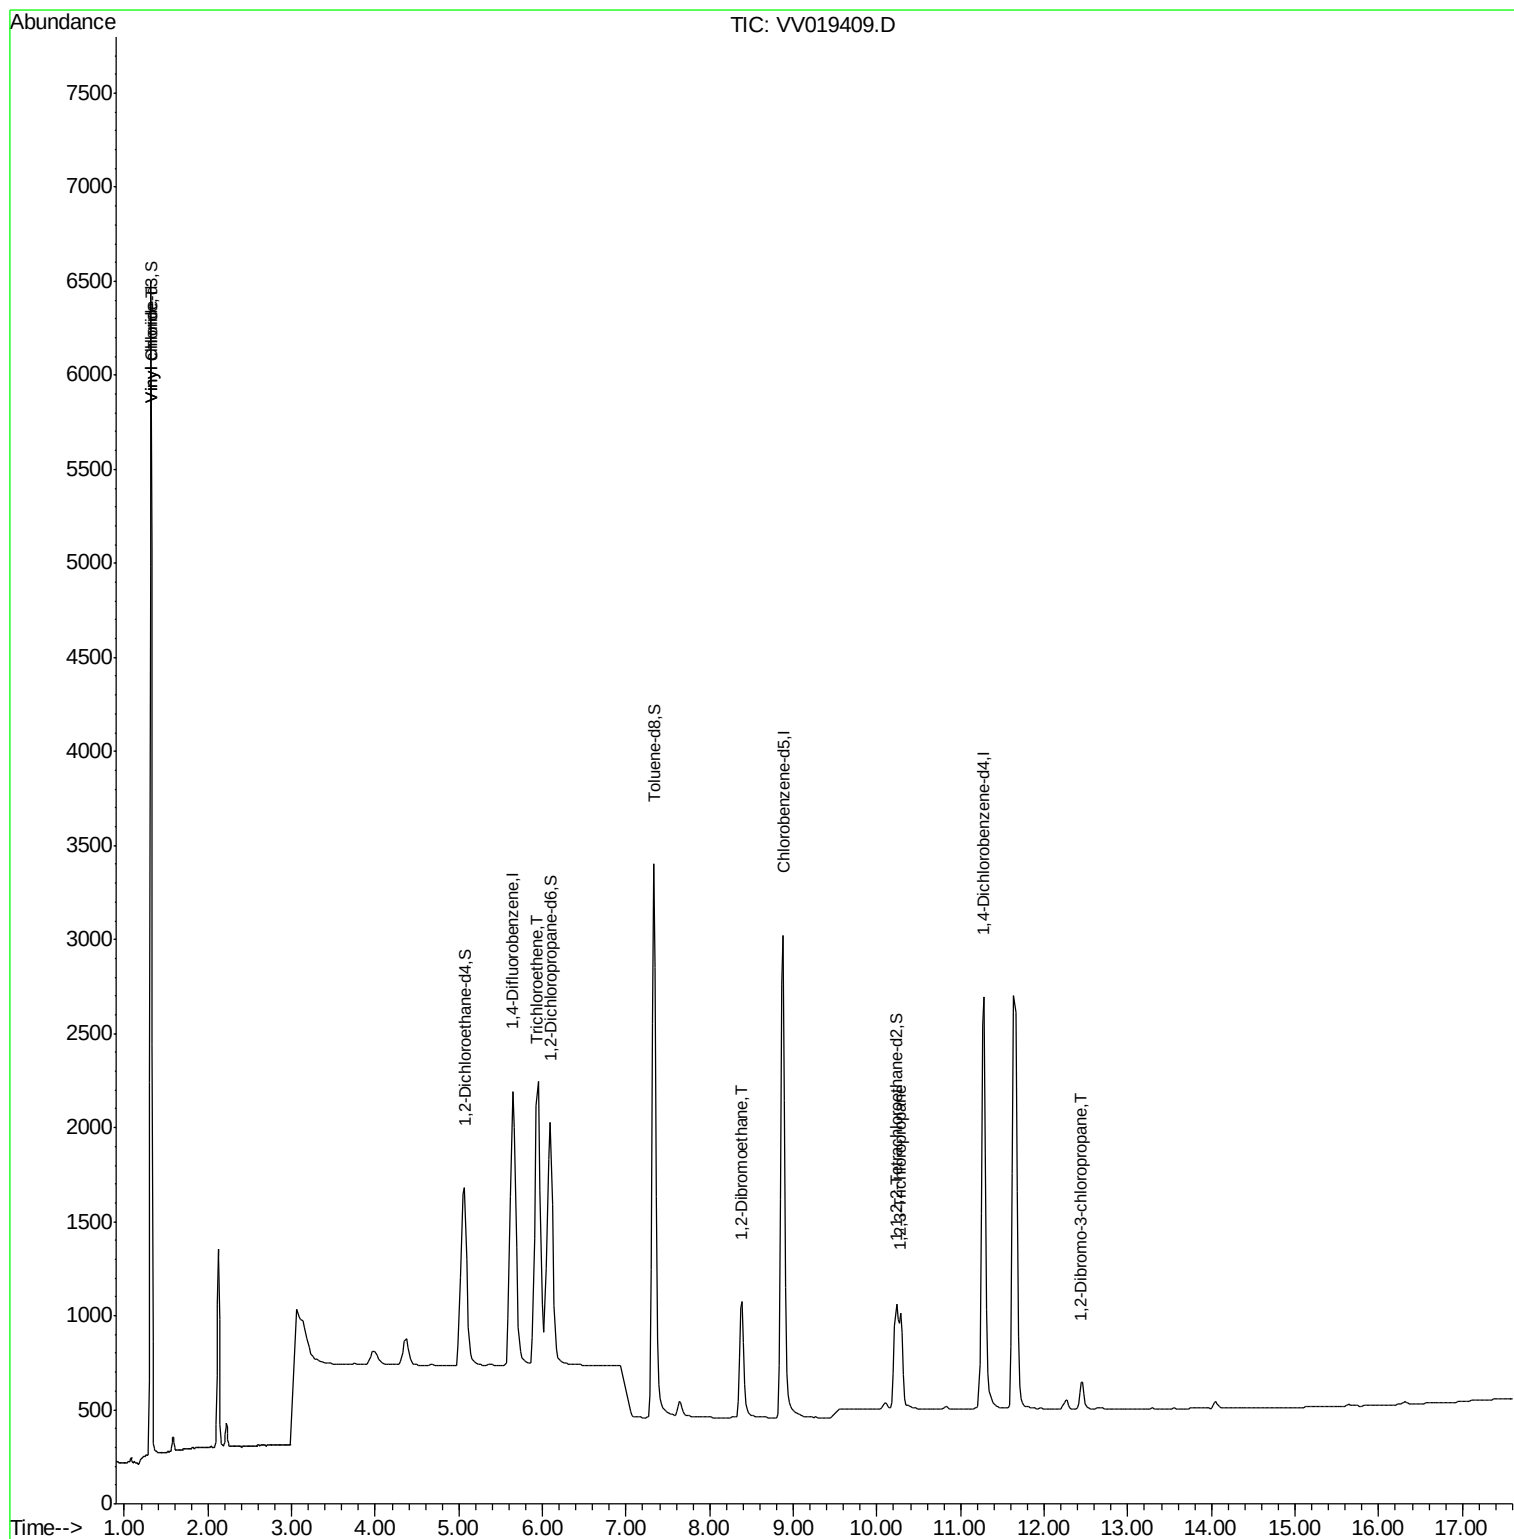

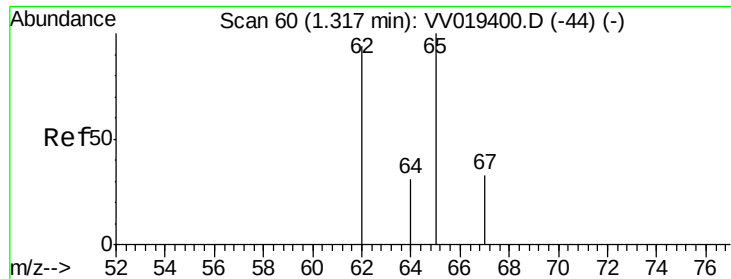

#3

Vinyl chloride

Concen: 0.484 ug/L

RT: 1.32 min Scan# 60

Delta R.T. -0.00 min

Lab File: VV019409.D

Acq: 20 Nov 2020 09:11

Instrument :

MSVOA_V

ClientSampleId :





BFB303

Tgt Ion: 62 Resp: 3224

Ion Ratio Lower Upper

62 100

64 35.2 25.1 46.7

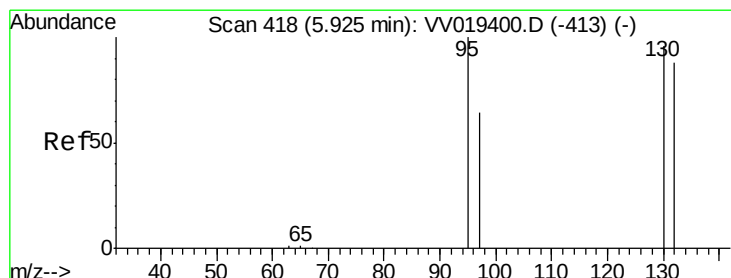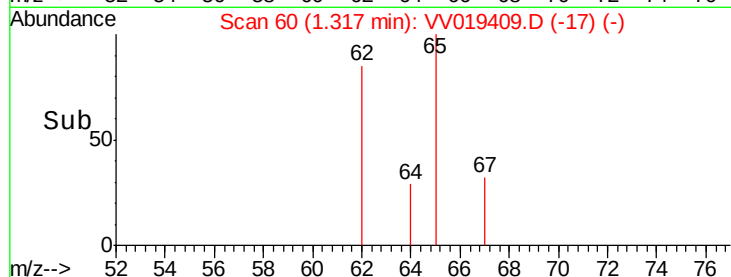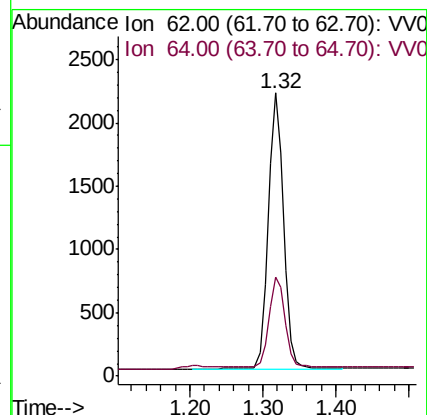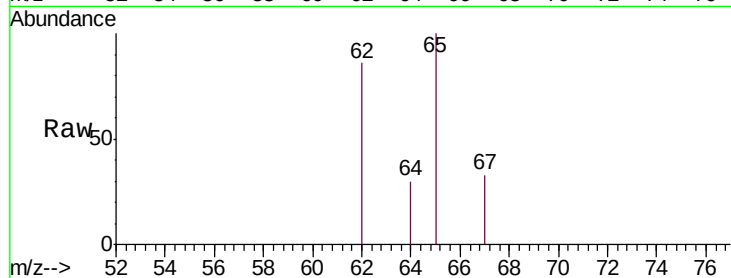

#6

Trichloroethene

Concen: 0.498 ug/L

RT: 5.93 min Scan# 418

Delta R.T. -0.00 min

Lab File: VV019409.D

Acq: 20 Nov 2020 09:11

Tgt Ion: 95 Resp: 1980




Ion Ratio Lower Upper


95 100

97 64.9 45.6 84.6

132 86.9 61.0 113.2

130 94.0 65.9 122.3

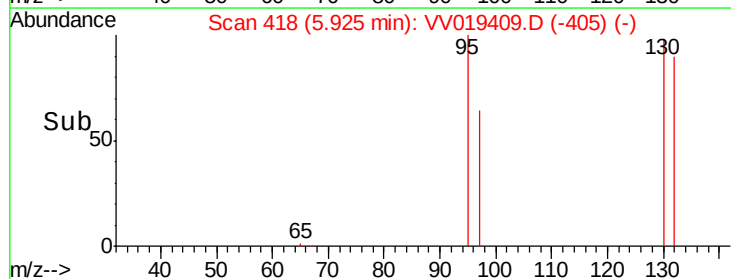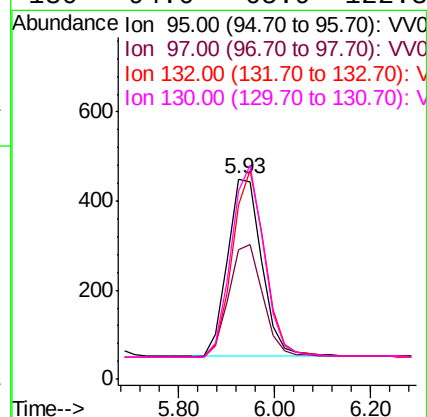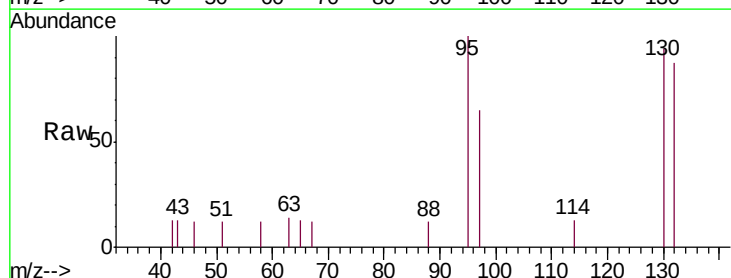

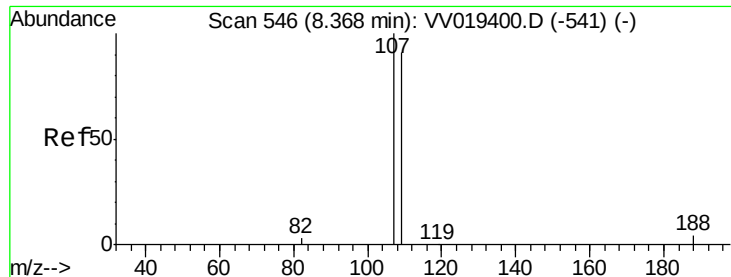

#9

1,2-Dibromoethane

Concen: 0.490 ug/L

RT: 8.38 min Scan# 547

Delta R.T. 0.02 min

Lab File: VV019409.D

Acq: 20 Nov 2020 09:11

Instrument :

MSVOA_V

ClientSampleId :

BFB303


Tgt Ion: 107 Resp: 1111

Ion Ratio Lower Upper

107 100

109 97.2 68.5 127.1




188 17.8 13.9 20.9

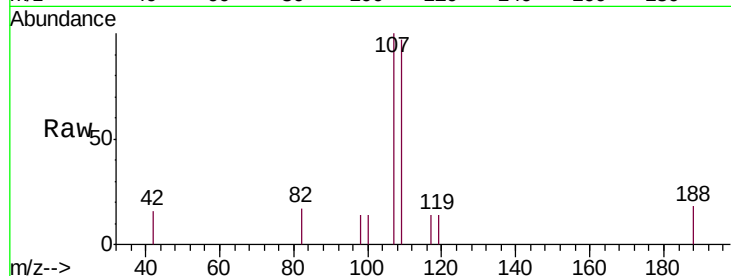

Abundance Ion 107.00 (106.70 to 107.70): V

Ion 109.00 (108.70 to 109.70): V

Ion 188.00 (187.70 to 188.70): V

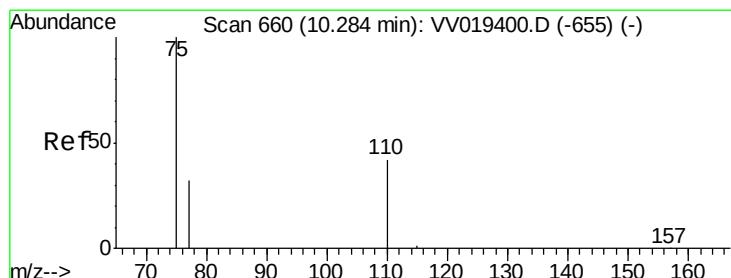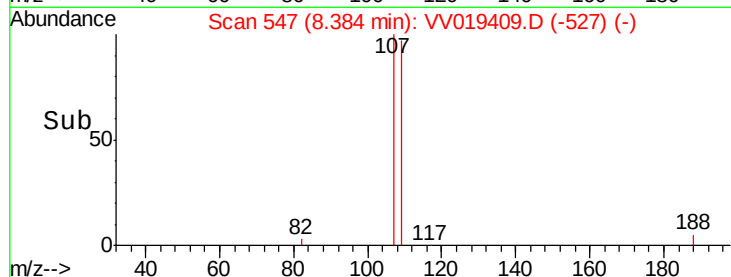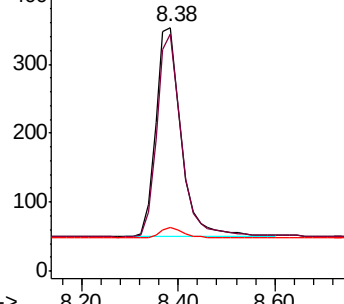

#12

1,2,3-Trichloropropane

Concen: 0.510 ug/L

RT: 10.28 min Scan# 660

Delta R.T. -0.00 min

Lab File: VV019409.D

Acq: 20 Nov 2020 09:11


Tgt Ion: 75 Resp: 936

Ion Ratio Lower Upper

75 100

110 43.9 34.5 51.7



77 33.4 25.7 38.5

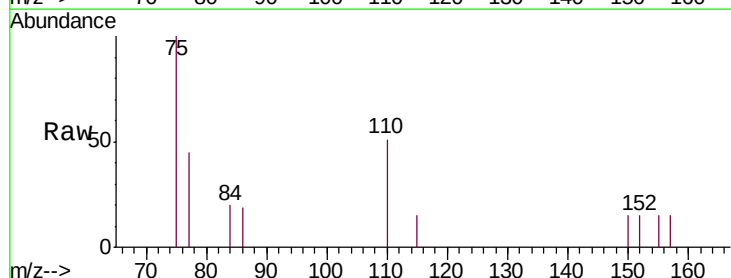


Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 110.00 (109.70 to 110.70): V

Ion 77.00 (76.70 to 77.70): VV0

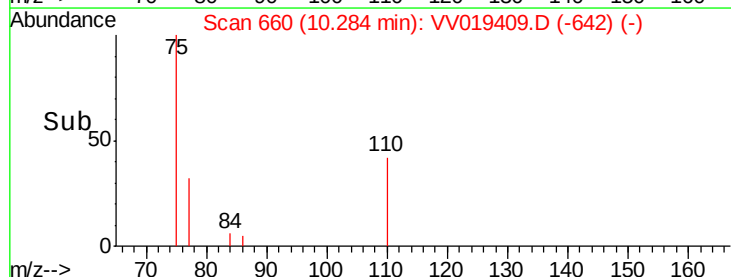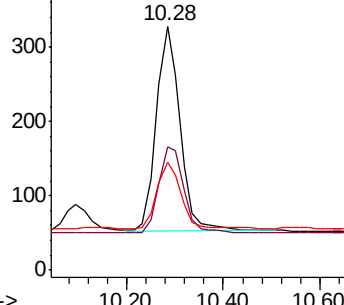

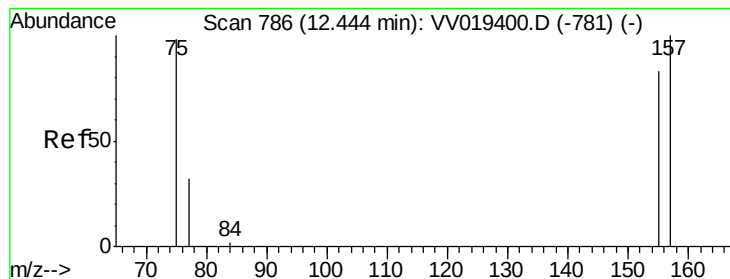

#13

1,2-Dibromo-3-chloropropane

Concen: 0.539 ug/L

RT: 12.44 min Scan# 786

Delta R.T. -0.00 min

Lab File: VV019409.D

Acq: 20 Nov 2020 09:11

Instrument :

MSVOA_V

ClientSampleId :

BFB303


Tgt Ion: 75 Resp: 160

Ion Ratio Lower Upper

75 100

157 99.0 79.2 118.8

155 89.6 71.0 106.6

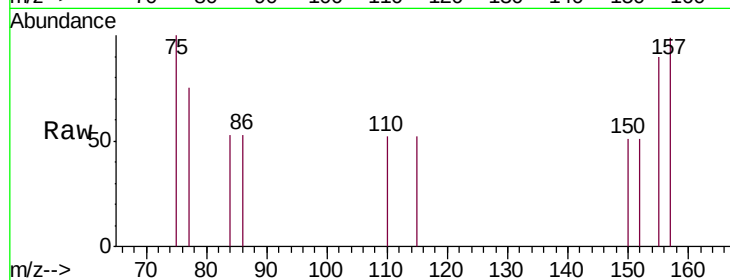

Abundance Ion 75.00 (74.70 to 75.70): VV019409.D (-768) (-)

Ion 157.00 (156.70 to 157.70): VV019409.D (-768) (-)

Ion 155.00 (154.70 to 155.70): VV019409.D (-768) (-)

