


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112020\
 Data File : VV019408.D
 Acq On : 20 Nov 2020 08:38
 Operator : SY/MD
 Sample : BFB65
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB303

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Nov 20 23:16:17 2020

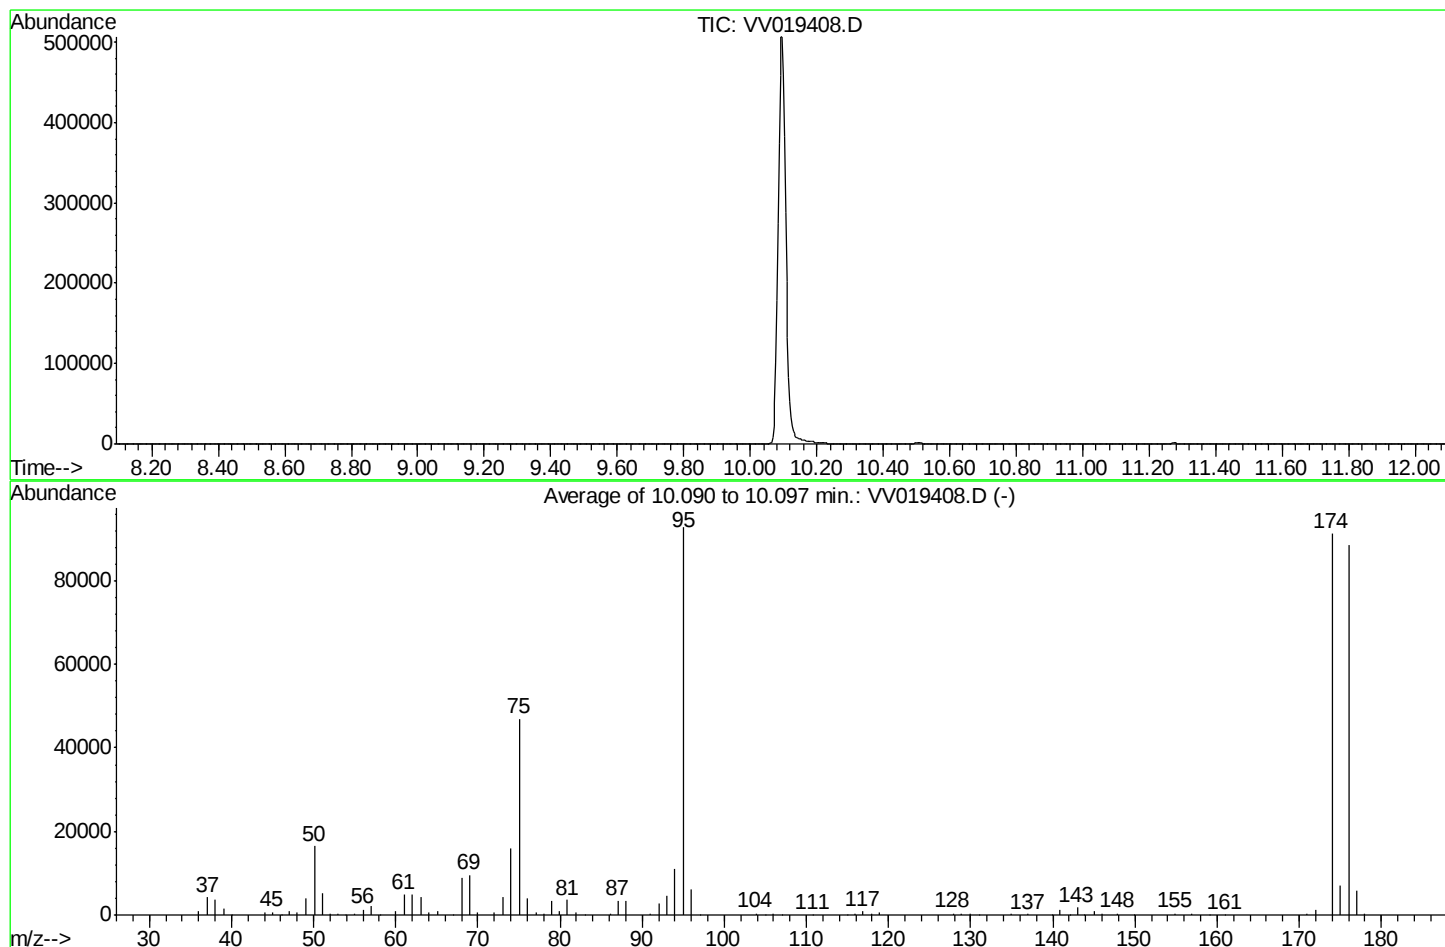

AutoFind: Scans 2799, 2800, 2801; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	16438	PASS
75	95	30	80	50.7	47034	PASS
95	95	100	100	100.0	92805	PASS
96	95	5	9	6.8	6267	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.3	91229	PASS
175	174	5	9	7.6	6962	PASS
176	174	95	101	96.9	88437	PASS
177	176	5	9	6.7	5883	PASS

m/z	Abundance
36.00	775.0
37.10	3949.0
38.00	3451.0
39.10	1505.0
40.10	192.0
44.00	685.0
45.00	663.0
46.10	146.0
47.10	805.0
48.00	569.0
49.00	3733.0
50.10	15370.0
51.10	4864.0
52.00	326.0
53.00	152.0
54.00	121.0
55.00	259.0
56.00	1161.0
57.00	2045.0
60.00	861.0
61.00	4598.0
62.00	4636.0
63.10	3970.0
64.00	733.0
65.00	1011.0
67.00	235.0
68.00	8379.0
69.00	8794.0
70.00	689.0
72.00	550.0
73.00	4162.0
74.00	15024.0
75.00	44672.0
76.00	4025.0
77.20	530.0
78.00	332.0
78.90	3346.0
79.90	819.0
80.90	3455.0
81.90	676.0
86.20	182.0
87.00	3332.0
88.00	3157.0
90.90	324.0
92.00	2531.0
93.00	4176.0
94.00	10381.0
95.00	87736.0
96.00	6133.0
97.00	178.0
103.90	334.0
105.00	135.0
105.90	378.0
107.00	109.0
110.80	106.0
115.00	105.0
116.00	367.0
116.90	795.0
117.90	404.0
118.90	643.0
127.80	379.0
128.90	217.0
129.90	348.0
131.00	157.0
134.80	189.0
137.00	202.0
140.00	103.0
140.90	943.0
142.10	105.0
143.00	1697.0
143.80	122.0
145.00	806.0
146.00	153.0
147.90	343.0
149.90	143.0
154.90	348.0
156.90	164.0
159.10	110.0
170.90	353.0
172.00	1120.0
174.00	83664.0
175.00	6474.0
176.00	81280.0
177.00	5572.0
177.90	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	832.0
37.10	4274.0
38.00	3761.0
39.10	1619.0
40.00	166.0
44.00	705.0
45.00	649.0
46.10	171.0
47.10	832.0
48.00	604.0
49.10	4009.0
50.10	16904.0
51.00	5488.0
52.00	338.0
53.00	186.0
53.90	116.0
55.00	293.0
56.00	1270.0
57.00	2330.0
60.00	954.0
61.00	4942.0
62.00	4923.0
63.10	4297.0
64.00	810.0
65.10	1074.0
68.00	9270.0
69.00	9941.0
70.00	759.0
72.00	510.0
73.00	4437.0
74.00	16520.0
75.10	48584.0
76.10	4242.0
77.20	642.0
78.10	369.0
78.90	3580.0
79.90	909.0
80.90	3770.0
81.90	721.0
86.20	222.0
87.00	3578.0
88.00	3430.0
90.90	309.0
92.00	2751.0
93.00	4730.0
94.00	11302.0
95.00	95904.0
96.00	6436.0
97.00	168.0
103.80	422.0
105.00	159.0
105.90	377.0
106.90	118.0
116.00	422.0
116.90	933.0
117.90	407.0
118.90	661.0
127.90	411.0
128.90	249.0
129.90	393.0
130.90	157.0
134.80	190.0
136.90	251.0
139.80	102.0
140.90	1145.0
142.10	132.0
142.90	1780.0
143.90	130.0
145.00	810.0
145.90	201.0
147.90	378.0
150.00	174.0
154.90	350.0
156.90	229.0
159.00	107.0
161.00	140.0
170.90	395.0
172.00	1329.0
174.00	94192.0
175.00	7237.0
176.00	91160.0
177.00	6074.0
177.90	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	798.0
37.10	4291.0
38.00	3755.0
39.10	1590.0
39.90	152.0
44.00	724.0
45.00	617.0
46.10	135.0
47.00	803.0
48.00	576.0
49.10	3853.0
50.10	17040.0
51.00	5513.0
52.00	302.0
53.00	169.0
55.00	244.0
56.00	1253.0
57.00	2455.0
58.10	117.0
60.00	1002.0
61.00	4953.0
62.00	4744.0
63.00	4313.0
64.00	783.0
65.10	1069.0
68.00	9349.0
69.00	9989.0
70.00	748.0
72.00	449.0
73.00	4397.0
74.00	16512.0
75.10	47848.0
76.10	4097.0
77.10	625.0
78.10	413.0
78.90	3582.0
79.90	891.0
80.90	3725.0
81.90	726.0
83.10	109.0
86.20	195.0
87.00	3464.0
88.00	3377.0
91.00	327.0
92.00	2745.0
93.00	4812.0
94.00	11190.0
95.10	94776.0
96.00	6232.0
97.10	123.0
103.80	463.0
104.90	174.0
105.90	357.0
106.90	129.0
115.90	445.0
116.90	981.0
118.00	442.0
118.90	648.0
127.90	408.0
128.90	241.0
129.90	405.0
130.90	136.0
134.90	211.0
136.90	254.0
140.90	1260.0
142.00	138.0
142.90	1656.0
143.90	122.0
145.00	738.0
145.90	243.0
147.90	321.0
150.00	162.0
154.90	350.0
156.90	261.0
158.90	129.0
160.90	133.0
170.90	367.0
172.00	1393.0
174.00	95832.0
175.00	7176.0
176.00	92872.0
177.00	6005.0
177.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

Scan 2787 (10.052 min): VV019408.D
BFB65

m/z	Abundance
39.90	153.0
44.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303