

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033029.D
 Acq On : 20 Nov 2023 18:12
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 20 23:42:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 20 23:40:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	283624	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	281290	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	149628	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	61401	41.405	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.820%		
7) Chloroethane-d5	1.532	69	48412	42.448	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.900%		
11) 1,1-Dichloroethene-d2	2.060	65	23635	38.952	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.900%		
21) 2-Butanone-d5	3.783	46	88393	93.686	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.690%		
24) Chloroform-d	4.249	84	156216	42.745	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.500%		
26) 1,2-Dichloroethane-d4	4.941	65	102244	44.850	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.700%		
32) Benzene-d6	4.960	84	281277	42.940	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.880%		
36) 1,2-Dichloropropane-d6	5.989	67	84762	45.632	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.260%		
41) Toluene-d8	7.246	98	241535	38.626	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.260%#		
43) trans-1,3-Dichloroprop...	7.555	79	44942	41.443	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.880%		
47) 2-Hexanone-d5	8.024	63	71693	93.270	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.270%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	120652	42.671	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.340%		
66) 1,2-Dichlorobenzene-d4	11.561	152	126013	47.227	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.460%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	2944	0.890	ug/L	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033029.D
Acq On : 20 Nov 2023 18:12
Operator : SY/MD
Sample : VIBLK
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 20 23:42:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 20 23:40:05 2023
Response via : Initial Calibration

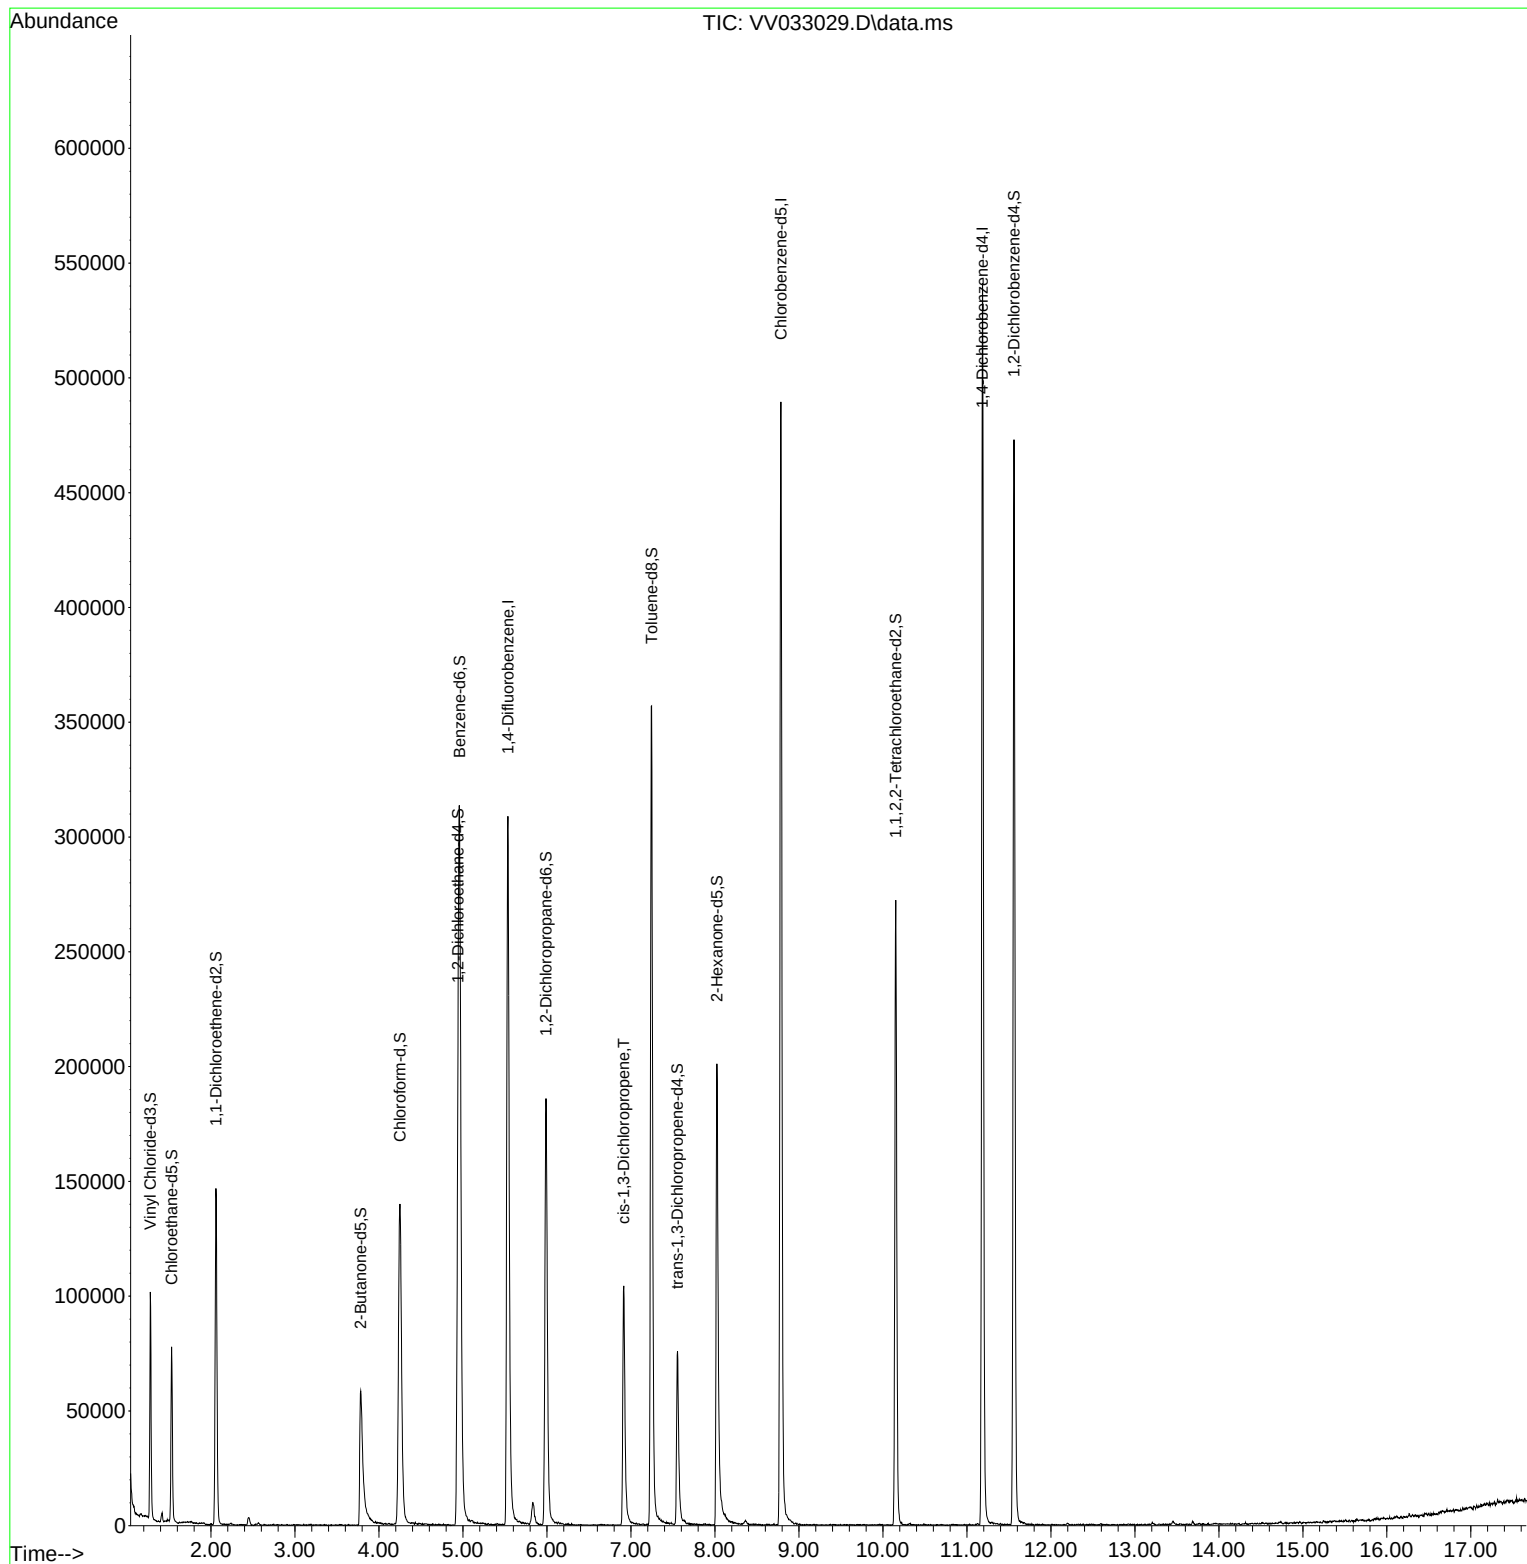

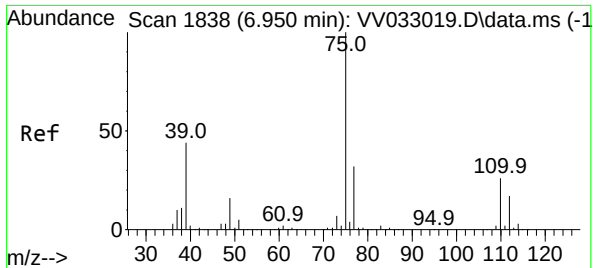

#39
 cis-1,3-Dichloropropene
 Concen: 0.890 ug/L
 RT: 6.915 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV033029.D
 Acq: 20 Nov 2023 18:12

Instrument :
 MSVOA_V
 ClientSampleId :

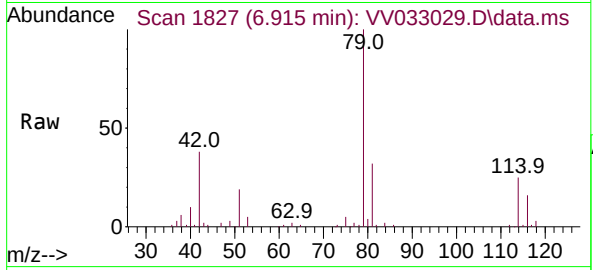

Tgt Ion:	75	Resp:	2944
Ion Ratio	Lower	Upper	
75	100		
77	46.0	21.9	40.7#

